

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020516\
 Data File : BF084895.D
 Acq On : 6 Feb 2016 7:37
 Operator : SJ/IZ
 Sample : H1320-15
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S4-B015(15-17)

Quant Time: Feb 08 00:43:27 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 03 14:16:01 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	176514	20.00	ng	-0.02
21) Naphthalene-d8	7.95	136	701389	20.00	ng	-0.02
38) Acenaphthene-d10	9.70	164	288554	20.00	ng	-0.03
63) Phenanthrene-d10	11.17	188	501801	20.00	ng	-0.03
75) Chrysene-d12	13.80	240	353574	20.00	ng	-0.03
86) Perylene-d12	15.17	264	327279	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	1056832	93.26	ng	-0.02
7) Phenol-d6	6.32	99	1409299	100.31	ng	-0.02
23) Nitrobenzene-d5	7.23	82	798781	64.15	ng	-0.03
41) 2,4,6-Tribromophenol	10.49	330	328759	109.23	ng	-0.03
44) 2-Fluorobiphenyl	9.02	172	1207576	65.27	ng	-0.03
78) Terphenyl-d14	12.76	244	1019087	65.31	ng	-0.03
Target Compounds						
49) Dimethylphthalate	9.42	163	223231	10.16	ng	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020516\
Data File : BF084895.D
Acq On : 6 Feb 2016 7:37
Operator : SJ/IZ
Sample : H1320-15
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4-B015(15-17)

Quant Time: Feb 08 00:43:27 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

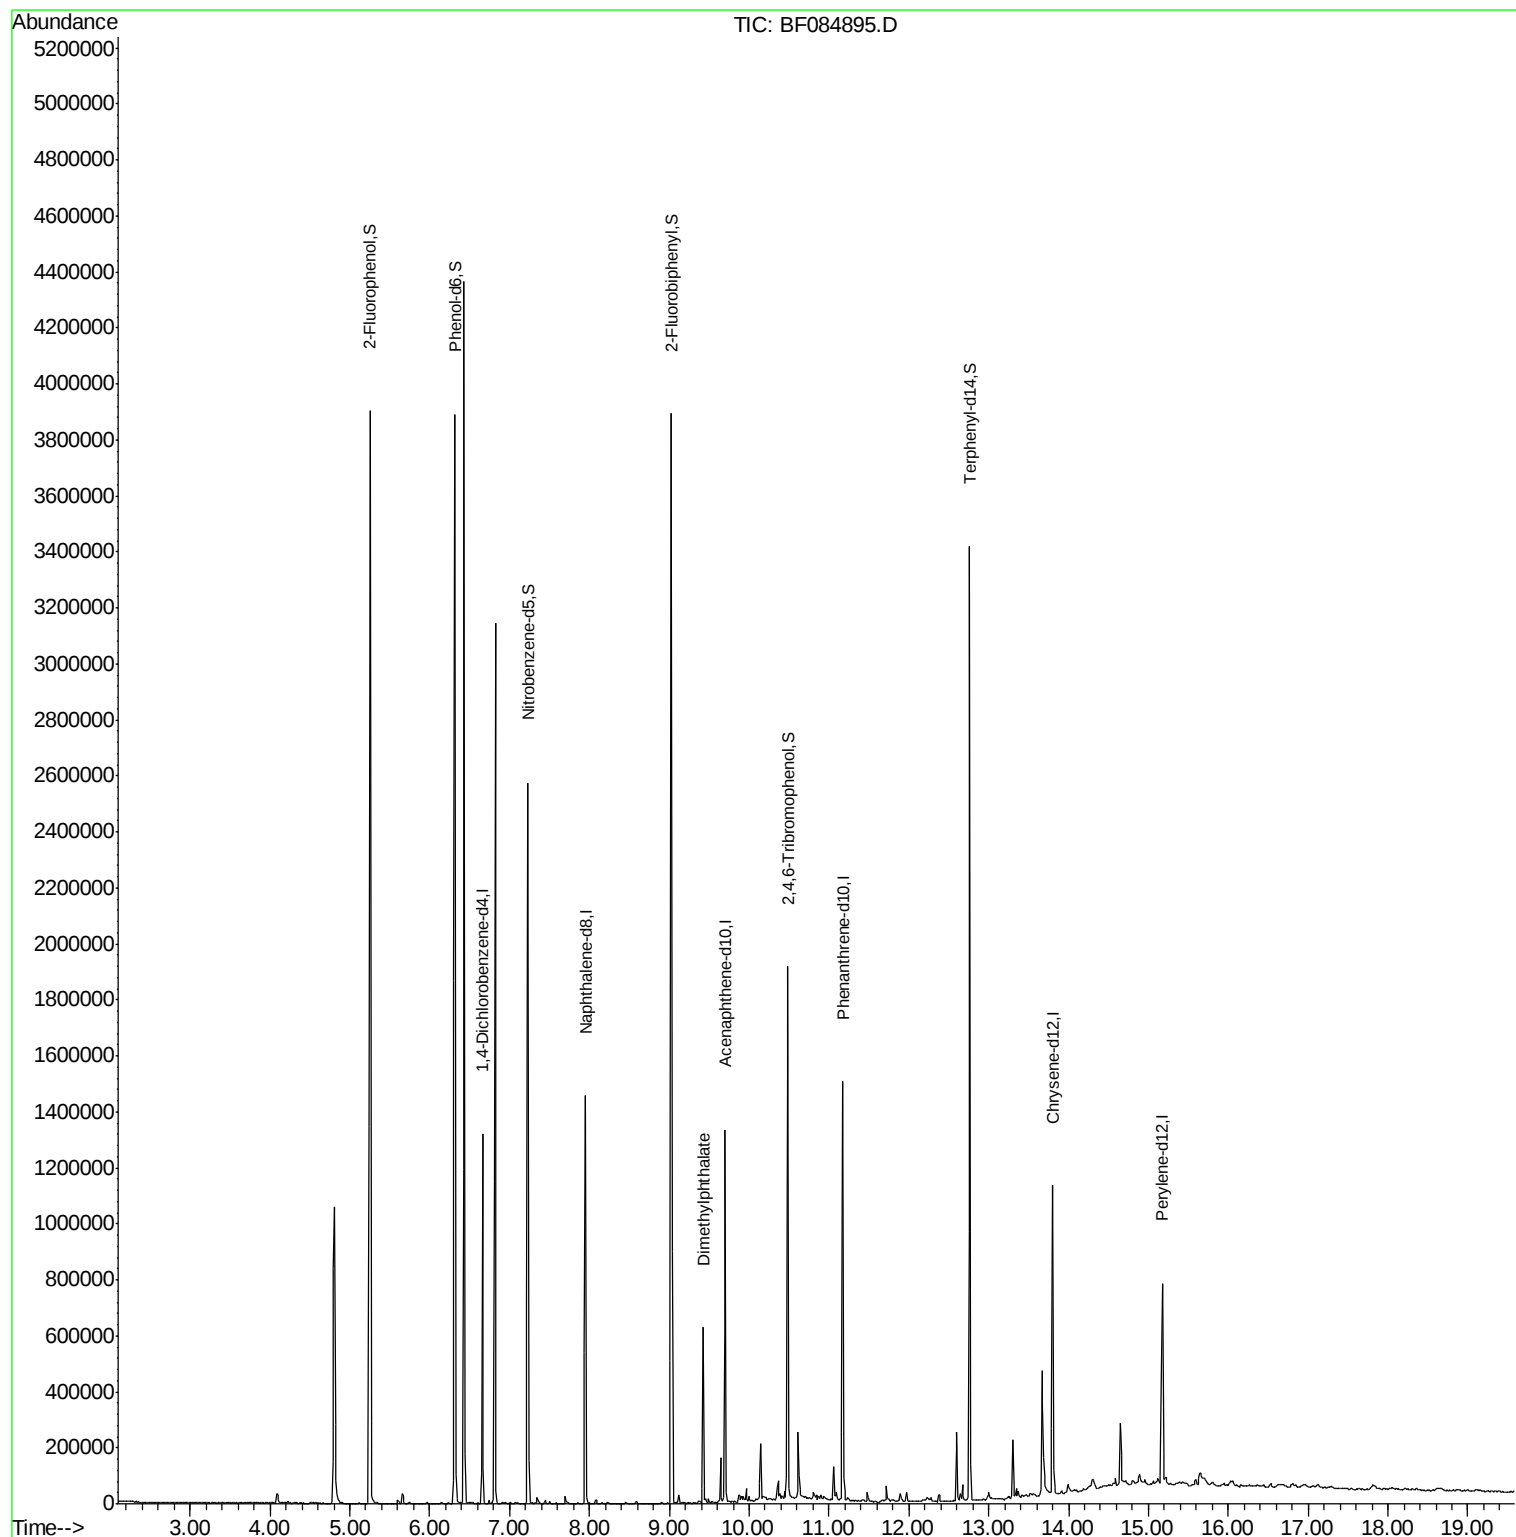

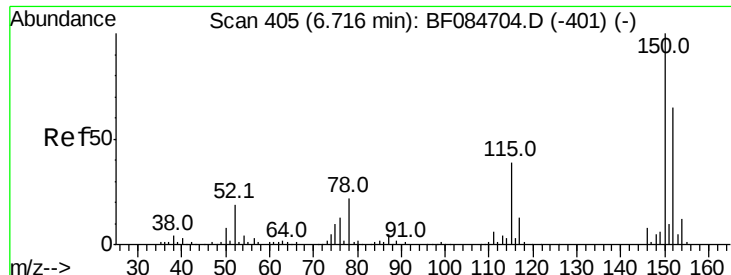

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.66 min Scan# 400

Delta R.T. -0.02 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37

Instrument :

BNA_F

ClientSampleId :

S4-B015(15-17)


Tot Ion:152 Resp: 176514

Ion Ratio Lower Upper

152 100

150 154.4 123.0 184.4




115 65.6 51.4 77.2

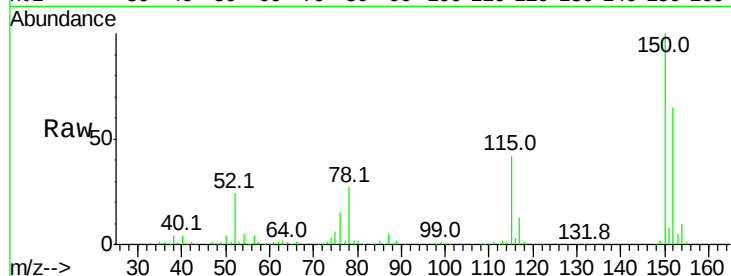

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

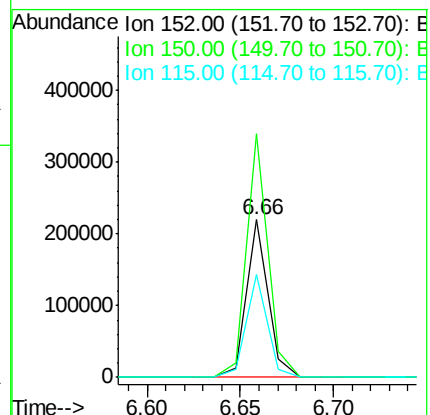

#5

2-Fluorophenol

Concen: 93.26 ng

RT: 5.25 min Scan# 277

Delta R.T. -0.02 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37


Tgt Ion:112 Resp: 1056832

Ion Ratio Lower Upper

112 100

64 63.2 36.6 55.0#



63 33.4 19.4 29.0#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

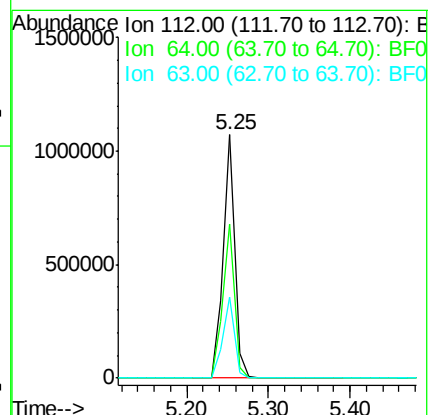

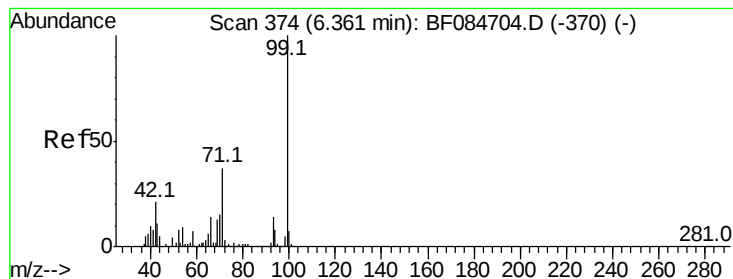

#7

Phenol-d6

Concen: 100.31 ng

RT: 6.32 min Scan# 370

Delta R.T. -0.02 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37

Instrument :





BNA_F

ClientSampleId :

S4-B015(15-17)

Tot Ion: 99 Resp: 1409299

Ion	Ratio	Lower	Upper
99	100		
42	19.4	12.8	19.2#
71	36.8	30.9	46.3

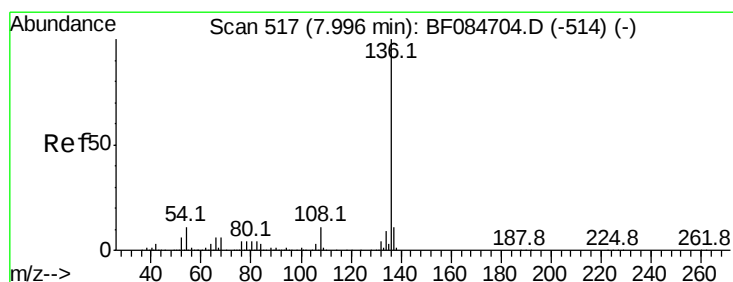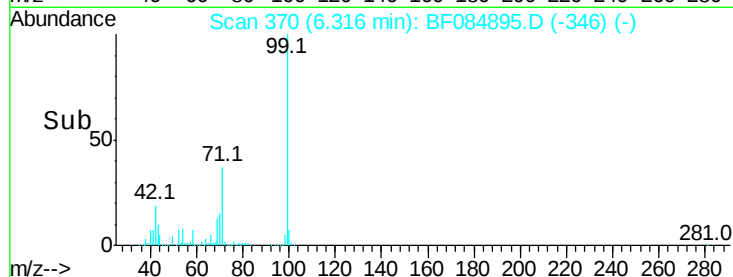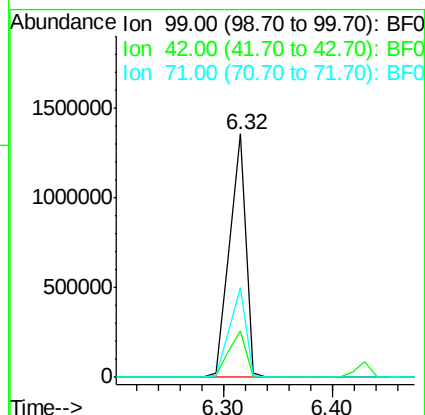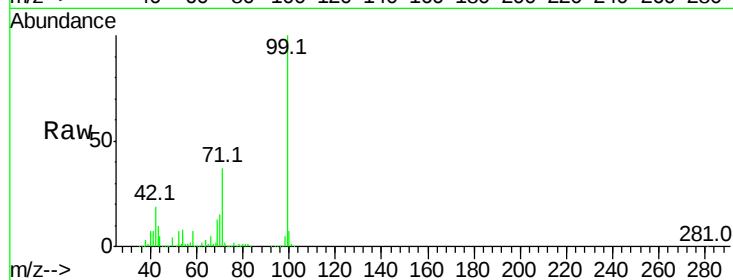

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 513




Delta R.T. -0.02 min


Lab File: BF084895.D

Acq: 6 Feb 2016 7:37

Tgt Ion: 136 Resp: 701389

Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.7	13.1
54	6.7	5.8	8.8
68	4.0	4.2	6.2#


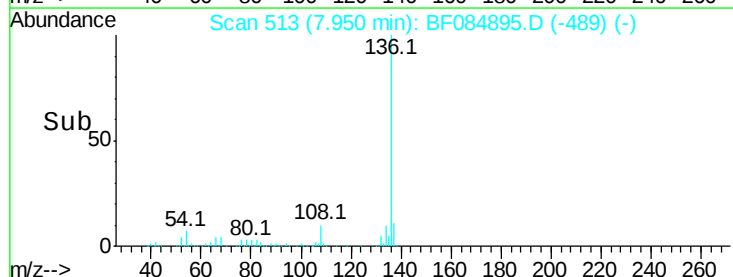
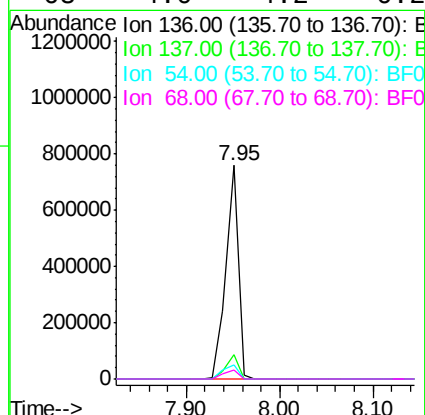
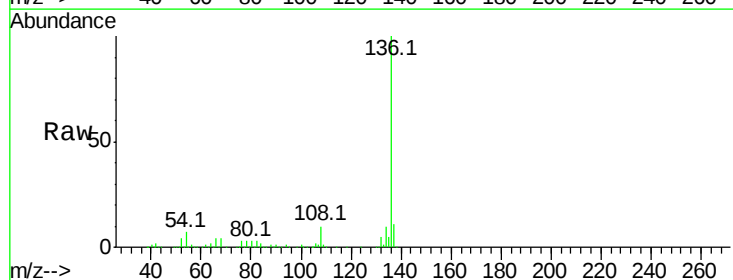




#23
 Nitrobenzene-d5
 Concen: 64.15 ng
 RT: 7.23 min Scan# 450
 Delta R.T. -0.03 min
 Lab File: BF084895.D
 Acq: 6 Feb 2016 7:37




Instrument :
 BNA_F
 ClientSampleId :
 S4-B015(15-17)


Tot Ion	82	Resp	798781
Ion Ratio	100		
128	42.4	34.6	51.8
54	57.4	38.4	57.6

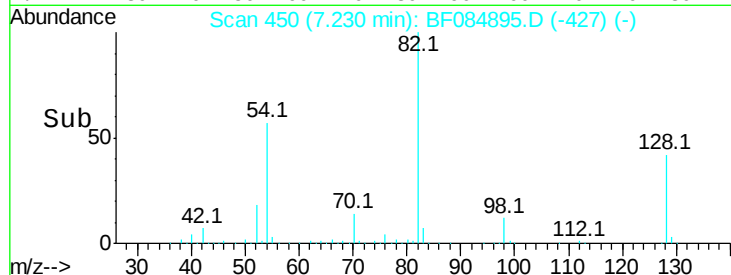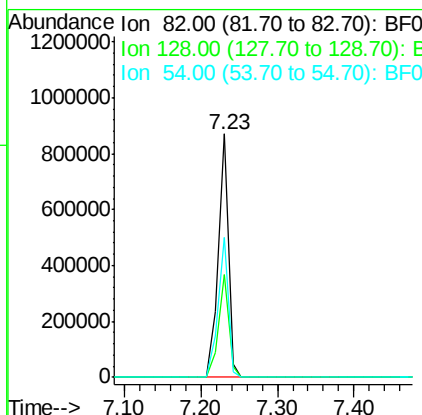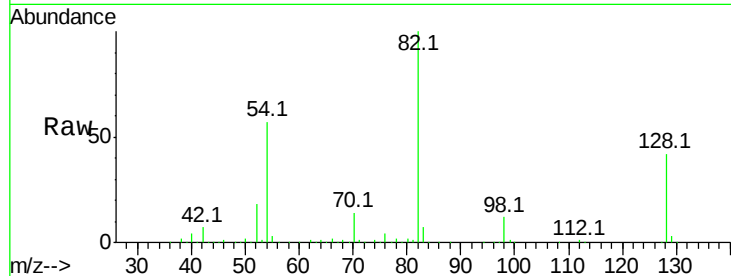

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.70 min Scan# 666
 Delta R.T. -0.03 min
 Lab File: BF084895.D
 Acq: 6 Feb 2016 7:37

Tgt Ion	164	Resp	288554
Ion Ratio	100		
162	107.4	85.1	127.7
160	48.6	37.5	56.3

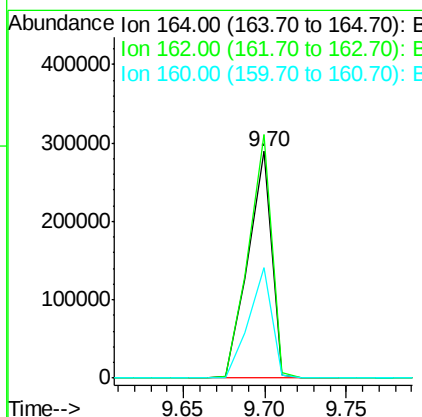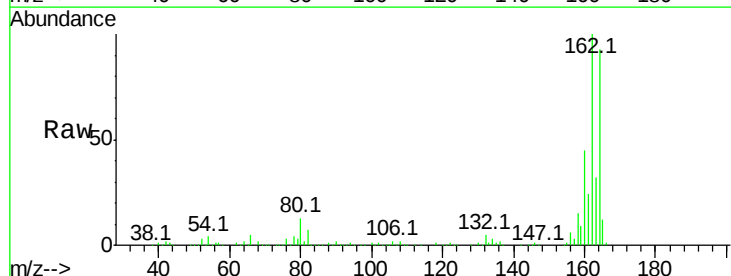


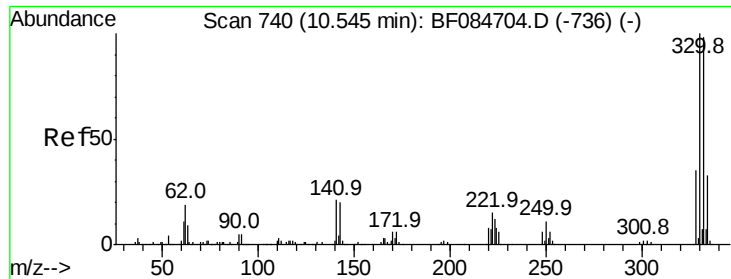




#41
 2,4,6-Tribromophenol
 Concen: 109.23 ng
 RT: 10.49 min Scan# 735
 Delta R.T. -0.03 min
 Lab File: BF084895.D
 Acq: 6 Feb 2016 7:37

Instrument :
 BNA_F
 ClientSampleId :
 S4-B015(15-17)

Tot Ion:330 Resp: 328759
 Ion Ratio Lower Upper
 330 100
 332 94.9 76.6 114.8
 141 32.0 27.8 41.6




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

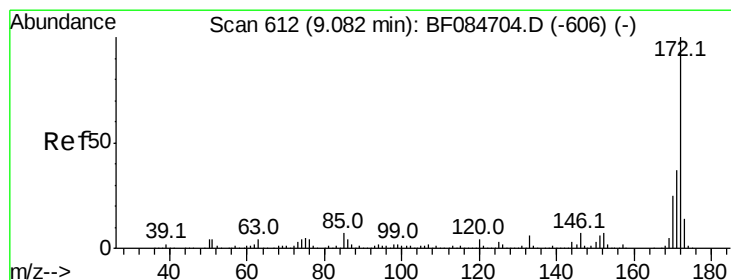
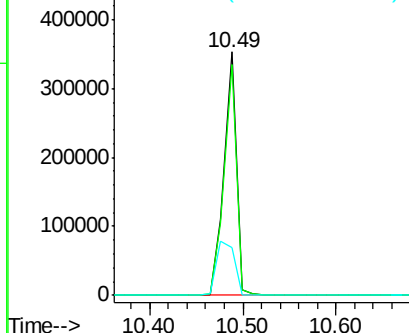



#44
 2-Fluorobiphenyl
 Concen: 65.27 ng
 RT: 9.02 min Scan# 607
 Delta R.T. -0.03 min
 Lab File: BF084895.D
 Acq: 6 Feb 2016 7:37

Tgt Ion:172 Resp: 1207576
 Ion Ratio Lower Upper
 172 100
 171 36.6 28.9 43.3
 170 24.8 18.6 27.8

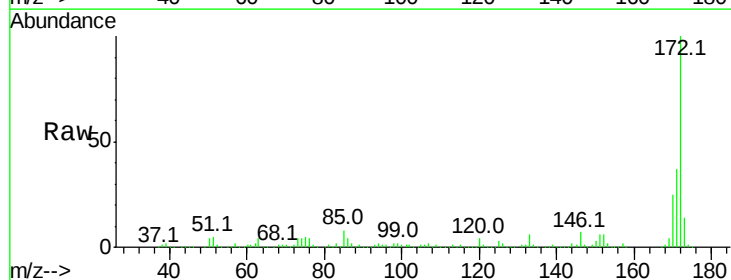

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

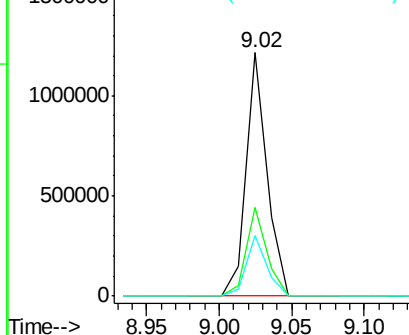

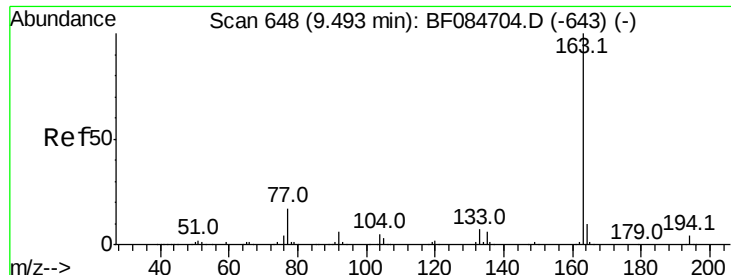

#49

Dimethylphthalate

Concen: 10.16 ng

RT: 9.42 min Scan# 642

Delta R.T. -0.05 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37

Instrument :

BNA_F

ClientSampleId :

S4-B015(15-17)


Tot Ion:163 Resp: 223231

Ion Ratio Lower Upper




163 100

194 2.7 8.0 12.0#

164 10.1 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

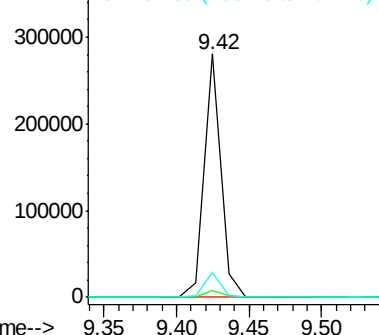

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.17 min Scan# 795

Delta R.T. -0.03 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37


Tgt Ion:188 Resp: 501801

Ion Ratio Lower Upper



188 100


94 8.3 9.0 13.4#

80 8.7 9.6 14.4#



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

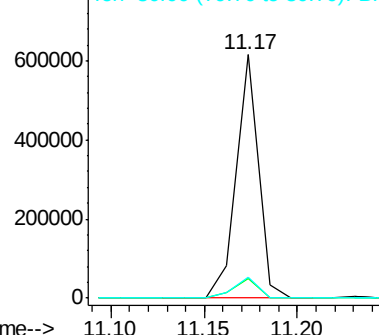



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.80 min Scan# 1025

Delta R.T. -0.03 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37

Instrument :

BNA_F

ClientSampleId :

S4-B015(15-17)


Tot Ion:240 Resp: 353574

Ion Ratio Lower Upper

240 100

120 9.9 9.5 14.3




236 25.6 20.6 31.0



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

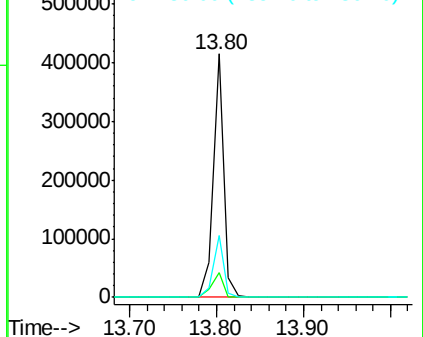

#78

Terphenyl-d14

Concen: 65.31 ng

RT: 12.76 min Scan# 934

Delta R.T. -0.03 min

Lab File: BF084895.D

Acq: 6 Feb 2016 7:37


Tgt Ion:244 Resp: 1019087

Ion Ratio Lower Upper

244 100

212 7.4 5.7 8.5



122 10.7 7.4 11.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

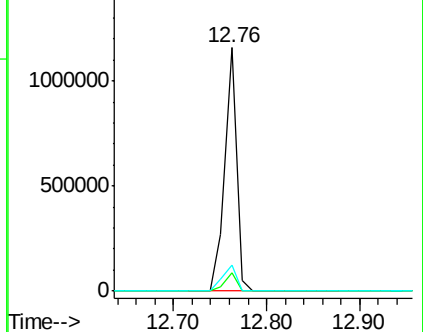


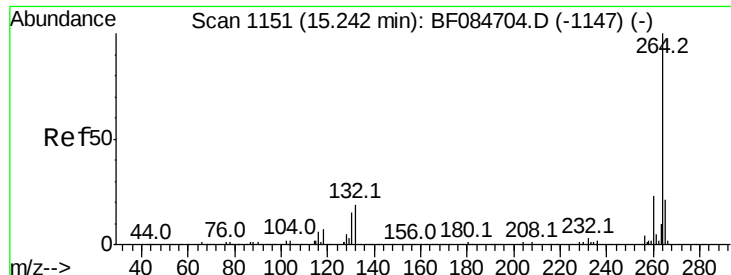

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.17 min Scan# 1145
Delta R.T. -0.03 min
Lab File: BF084895.D
Acq: 6 Feb 2016 7:37

Instrument :
BNA_F
ClientSampleId :
S4-B015(15-17)

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.4	29.2
265	21.7	17.8	26.6



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

