


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020516\
 Data File : BF084853.D
 Acq On : 5 Feb 2016 10:42
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 14:16:01 2016

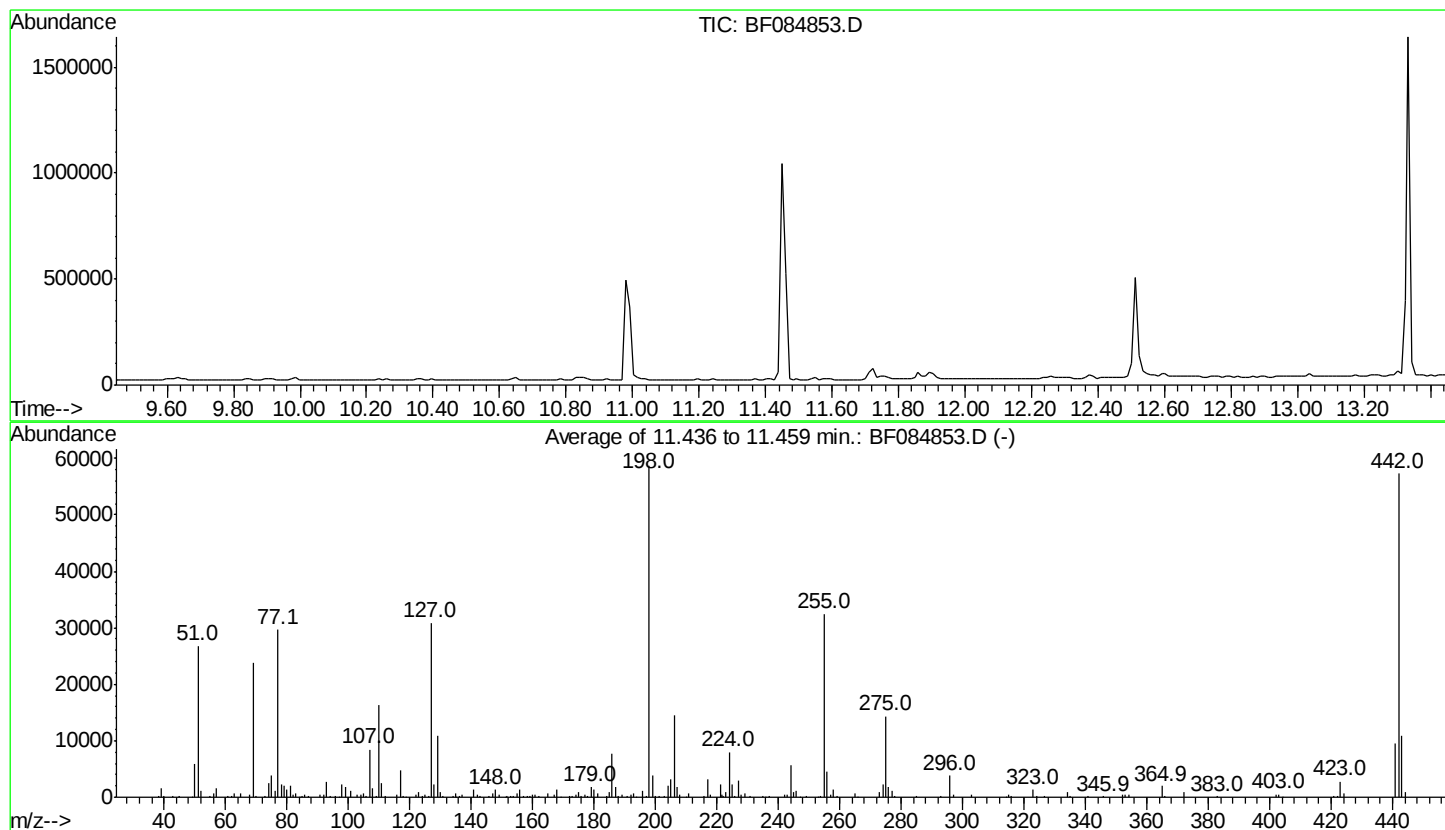

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	26860	PASS
68	69	0.00	2	1.6	387	PASS
69	198	0.00	100	40.4	23730	PASS
70	69	0.00	2	0.6	135	PASS
127	198	10	80	52.7	30938	PASS
197	198	0.00	2	0.4	252	PASS
198	198	100	100	100.0	58712	PASS
199	198	5	9	6.6	3901	PASS
275	198	10	60	24.4	14309	PASS
365	198	1	100	3.3	1960	PASS
441	442	0.01	24	16.6	9495	PASS
442	198	50	100	97.6	57282	PASS
443	442	15	24	19.1	10915	PASS