


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020516\
 Data File : BF084876.D
 Acq On : 5 Feb 2016 22:52
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 14:16:01 2016

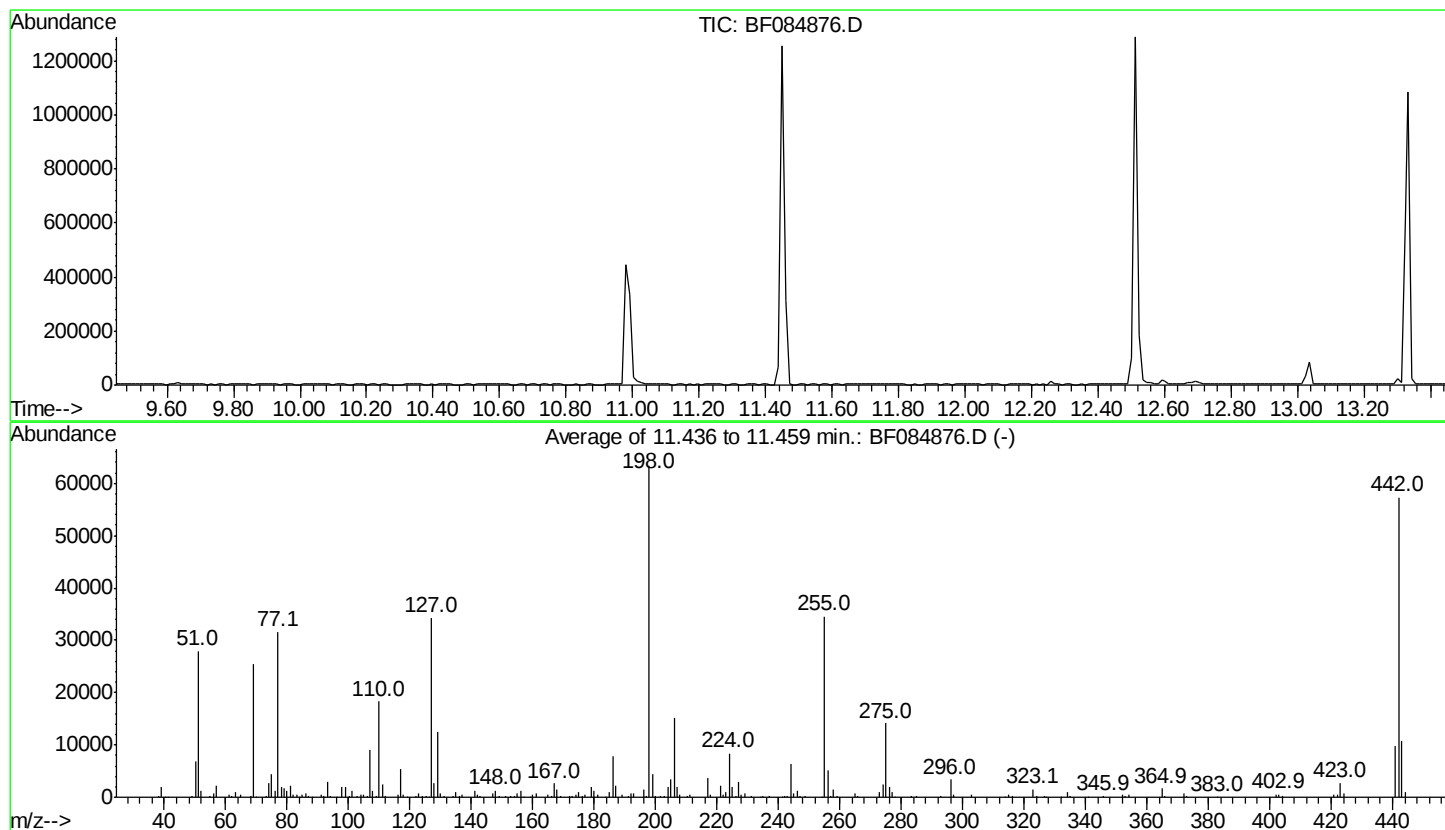

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	27911	PASS
68	69	0.00	2	1.2	311	PASS
69	198	0.00	100	40.3	25542	PASS
70	69	0.00	2	0.5	125	PASS
127	198	10	80	54.1	34269	PASS
197	198	0.00	2	0.6	350	PASS
198	198	100	100	100.0	63374	PASS
199	198	5	9	7.0	4422	PASS
275	198	10	60	22.3	14108	PASS
365	198	1	100	2.7	1703	PASS
441	442	0.01	24	17.0	9743	PASS
442	198	50	100	90.4	57316	PASS
443	442	15	24	18.8	10798	PASS