
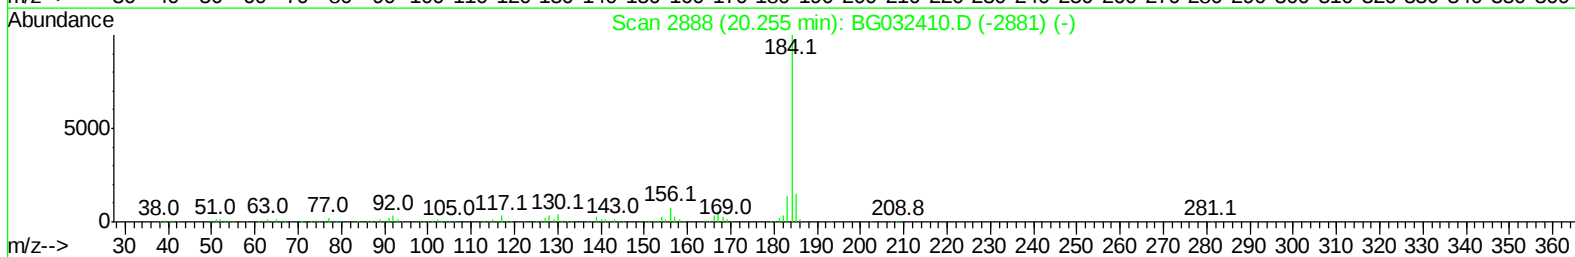
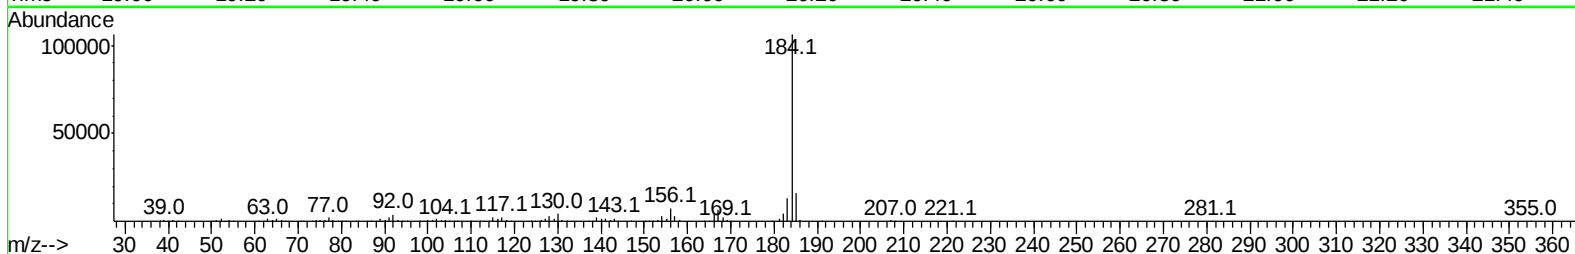


Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\  
Data File : BG032534.D  
Acq On : 5 Feb 2018 15:15  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:34:39 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 29 15:32:55 2018  
Response via : Initial Calibration

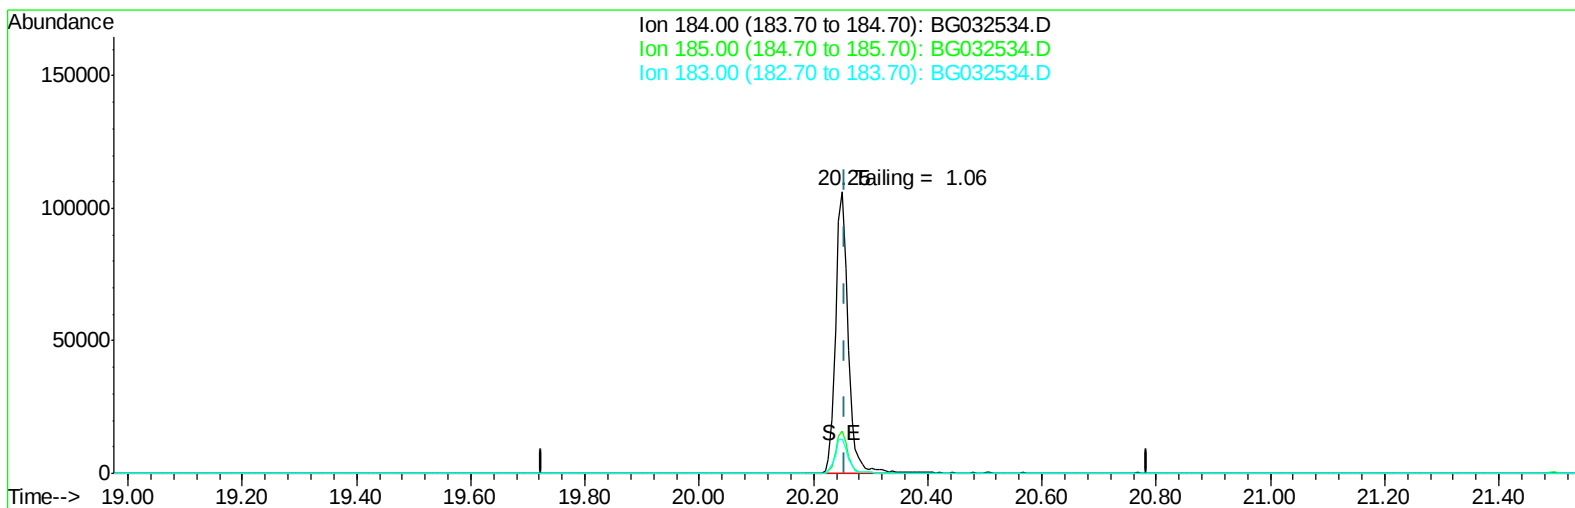

TIC: BG032534.D

(76) Benzidine

20.250min (-0.005) 56791.94ng

response 160584

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.99 |
| 183.00 | 13.30 | 12.36 |
| 0.00   | 0.00  | 0.00  |