
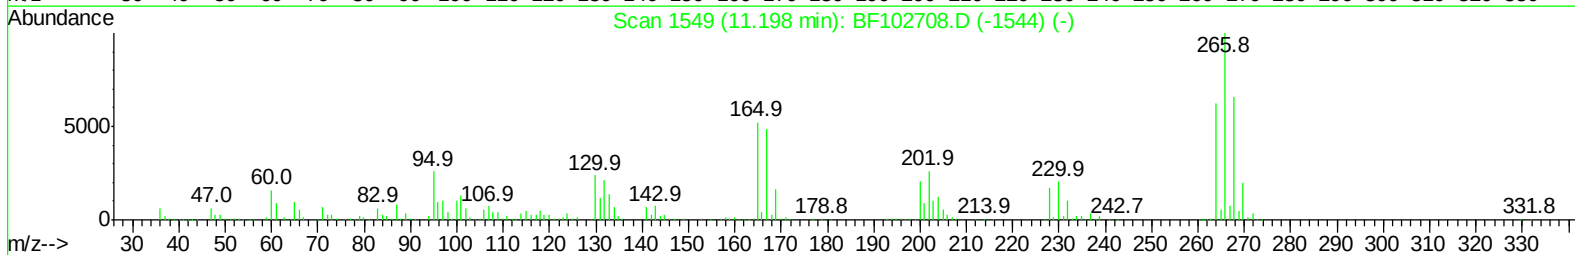
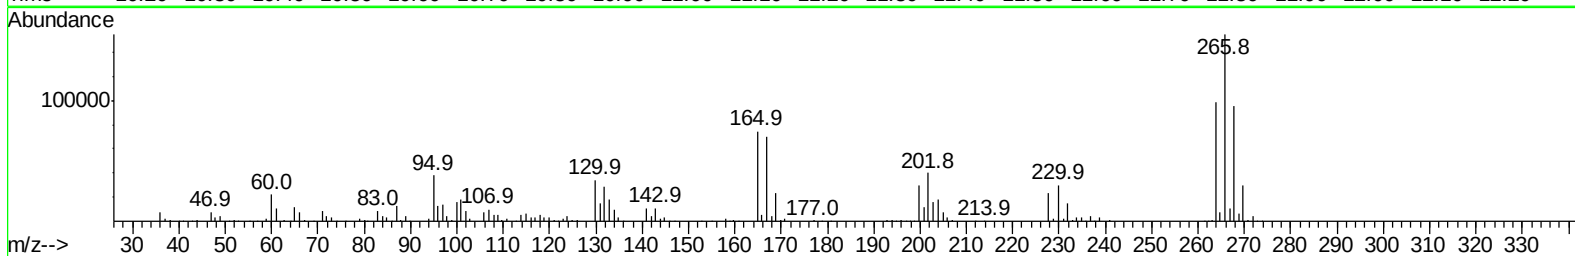


Data Path : U:\HPCHEM1\BNA F\DATA\BF020518\
Data File : BF102726.D
Acq On : 5 Feb 2018 9:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:11:38 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

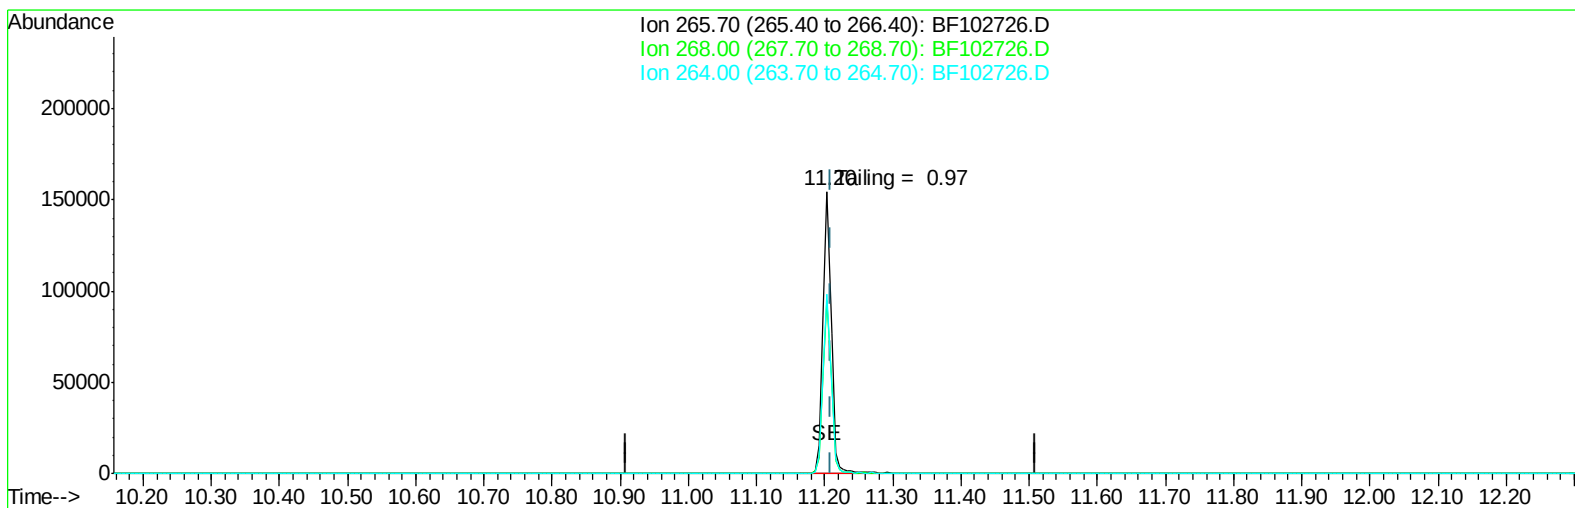

TIC: BF102726.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 71271.52ng

response 125964

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.54
264.00	61.90	63.72
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF020518\
 Data File : BF102726.D
 Acq On : 5 Feb 2018 9:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:11:38 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 12:44:16 2018
 Response via : Initial Calibration

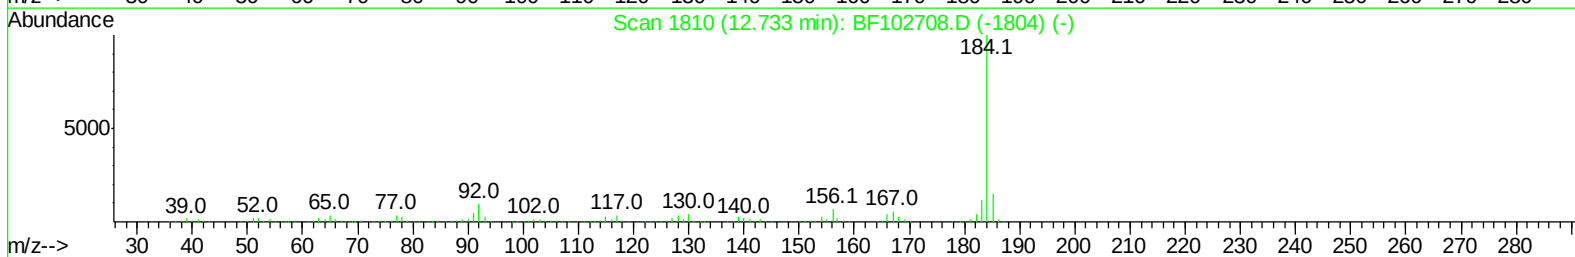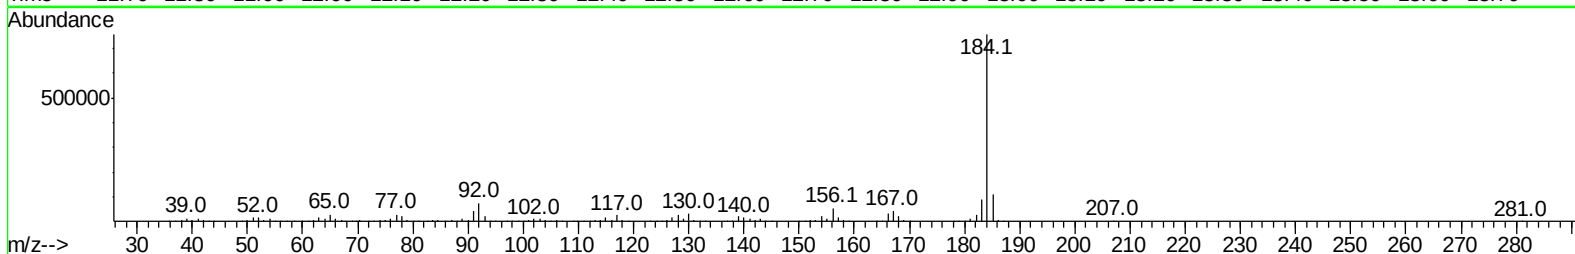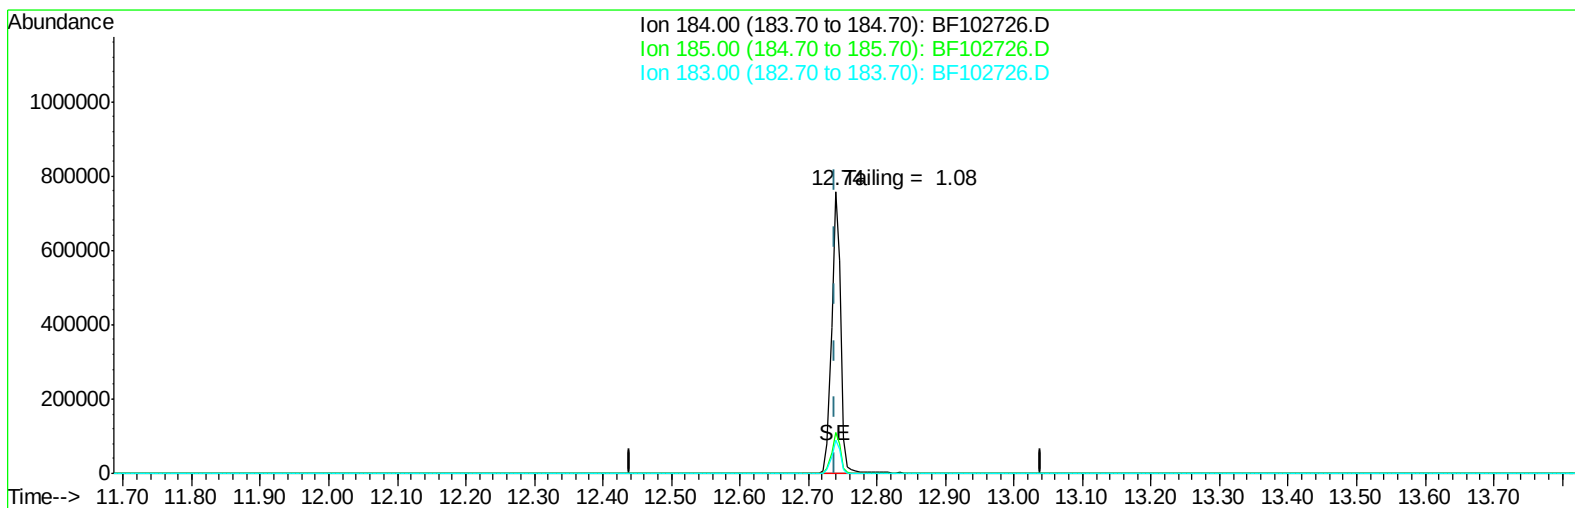

TIC: BF102726.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 691507

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.43
183.00	11.60	11.91
0.00	0.00	0.00