
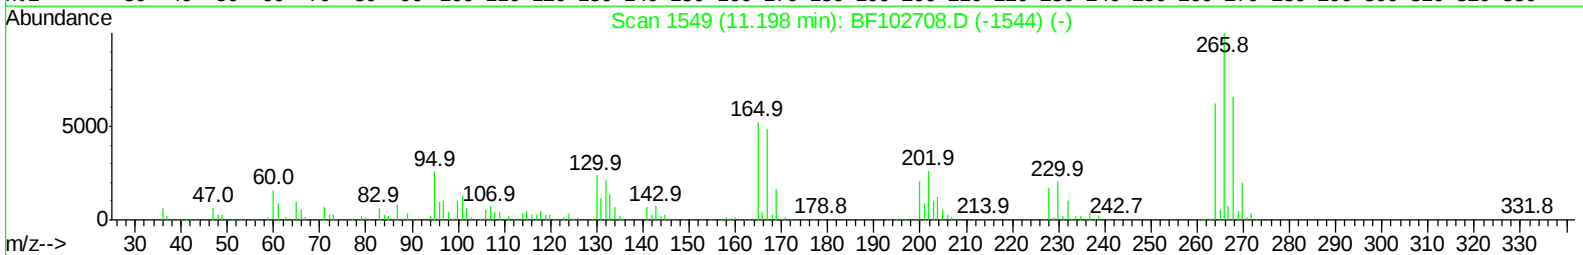
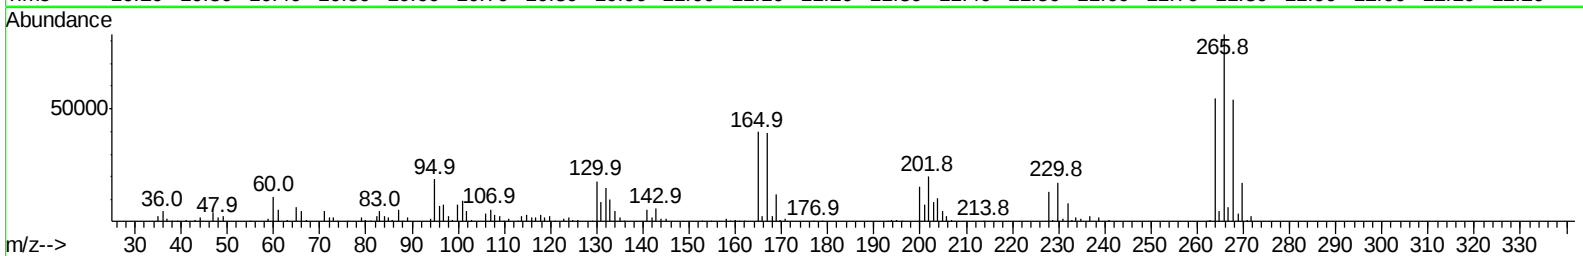


Data Path : U:\HPCHEM1\BNA F\DATA\BF020518\
Data File : BF102752.D
Acq On : 5 Feb 2018 22:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:12:44 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

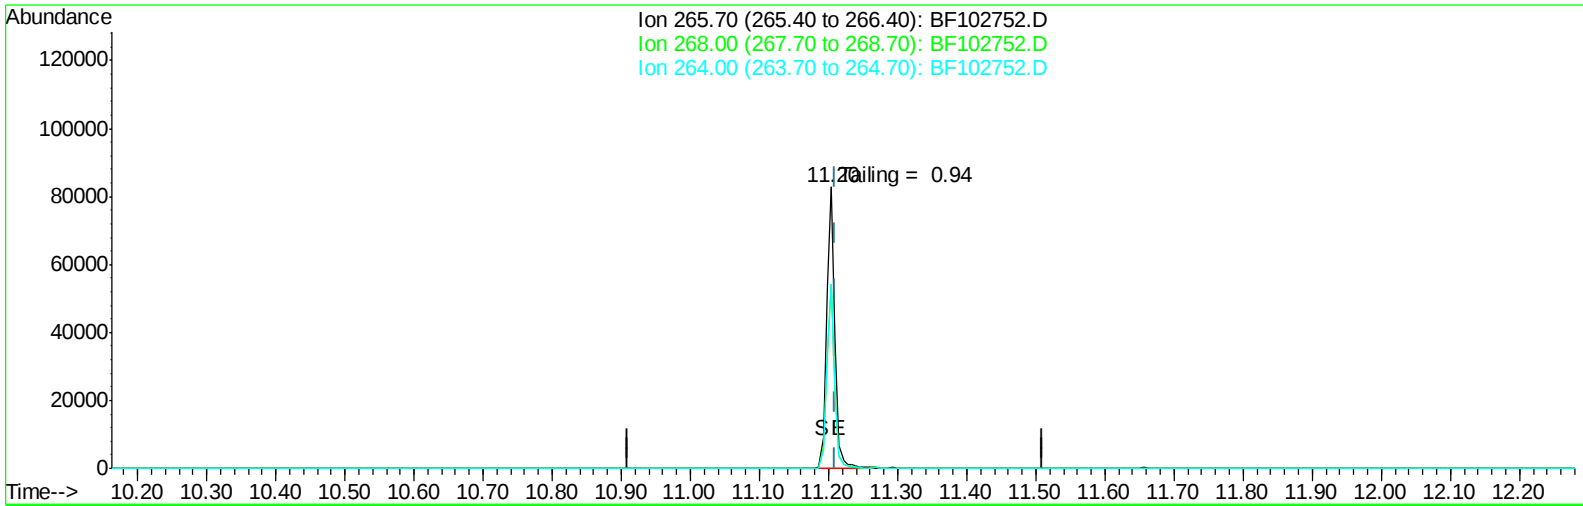

TIC: BF102752.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 25688.53ng

response 69334

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.29
264.00	61.90	65.66
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF020518\
Data File : BF102752.D
Acq On : 5 Feb 2018 22:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:12:44 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

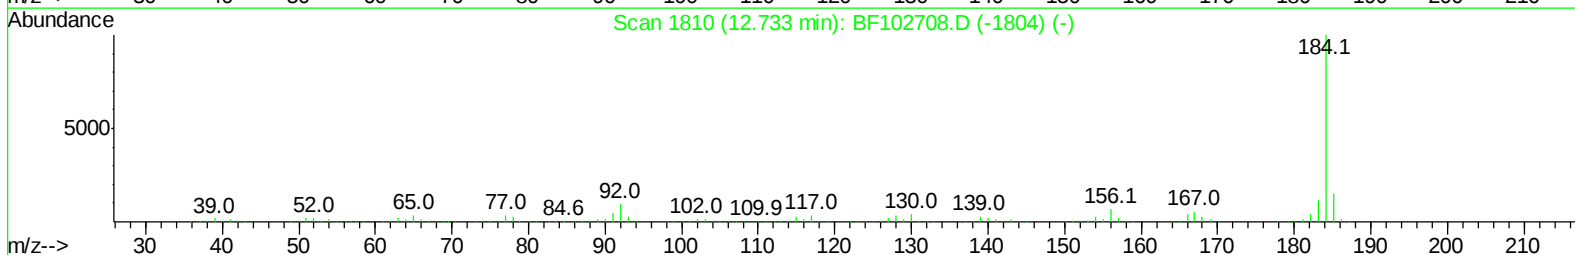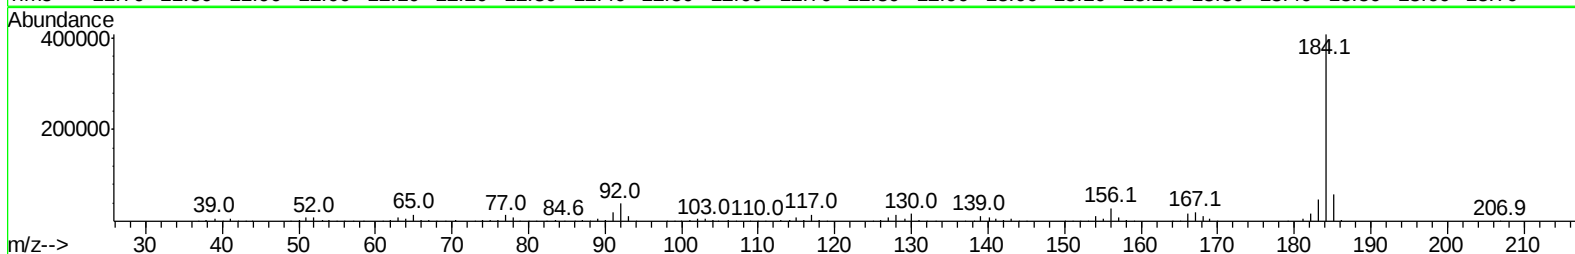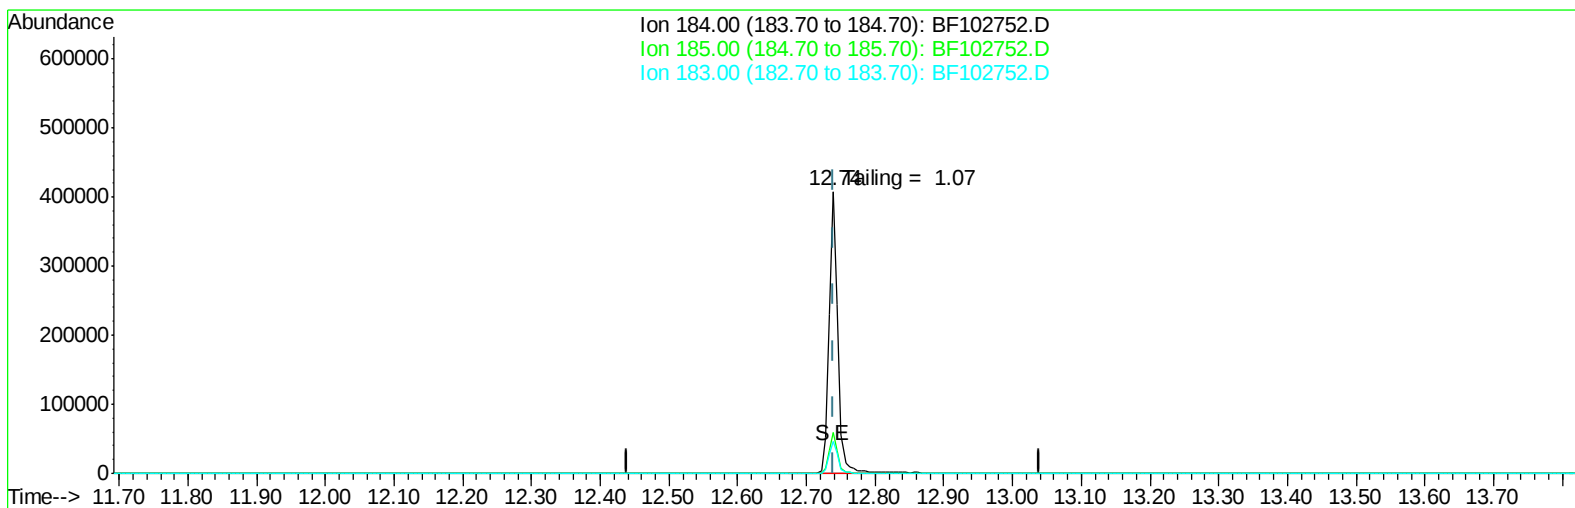

TIC: BF102752.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 369875

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.68
183.00	11.60	11.43
0.00	0.00	0.00