


Data Path : U:\HPCHEM1\BNA F\Data\BF020518\
 Data File : BF102726.D
 Acq On : 5 Feb 2018 9:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

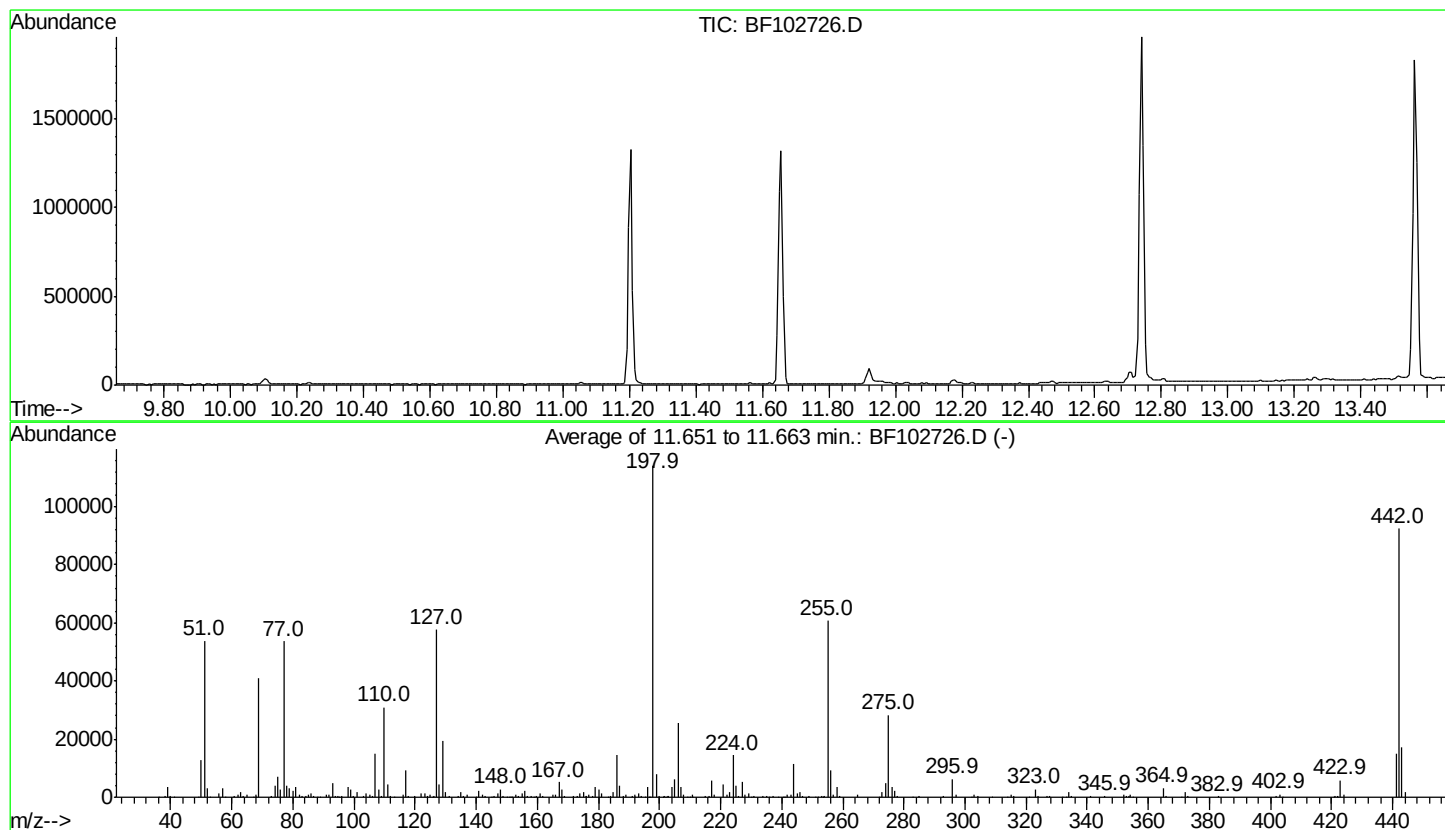

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	53879	PASS
68	69	0.00	2	1.9	783	PASS
69	198	0.00	100	36.0	41077	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	57496	PASS
197	198	0.00	2	0.2	193	PASS
198	198	100	100	100.0	114061	PASS
199	198	5	9	6.8	7725	PASS
275	198	10	60	24.9	28370	PASS
365	198	1	100	2.8	3192	PASS
441	443	0.01	100	87.9	14960	PASS
442	198	50	100	80.9	92328	PASS
443	442	15	24	18.4	17022	PASS