


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020520\
 Data File : BF118821.D
 Acq On : 5 Feb 2020 10:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 03 16:26:03 2020

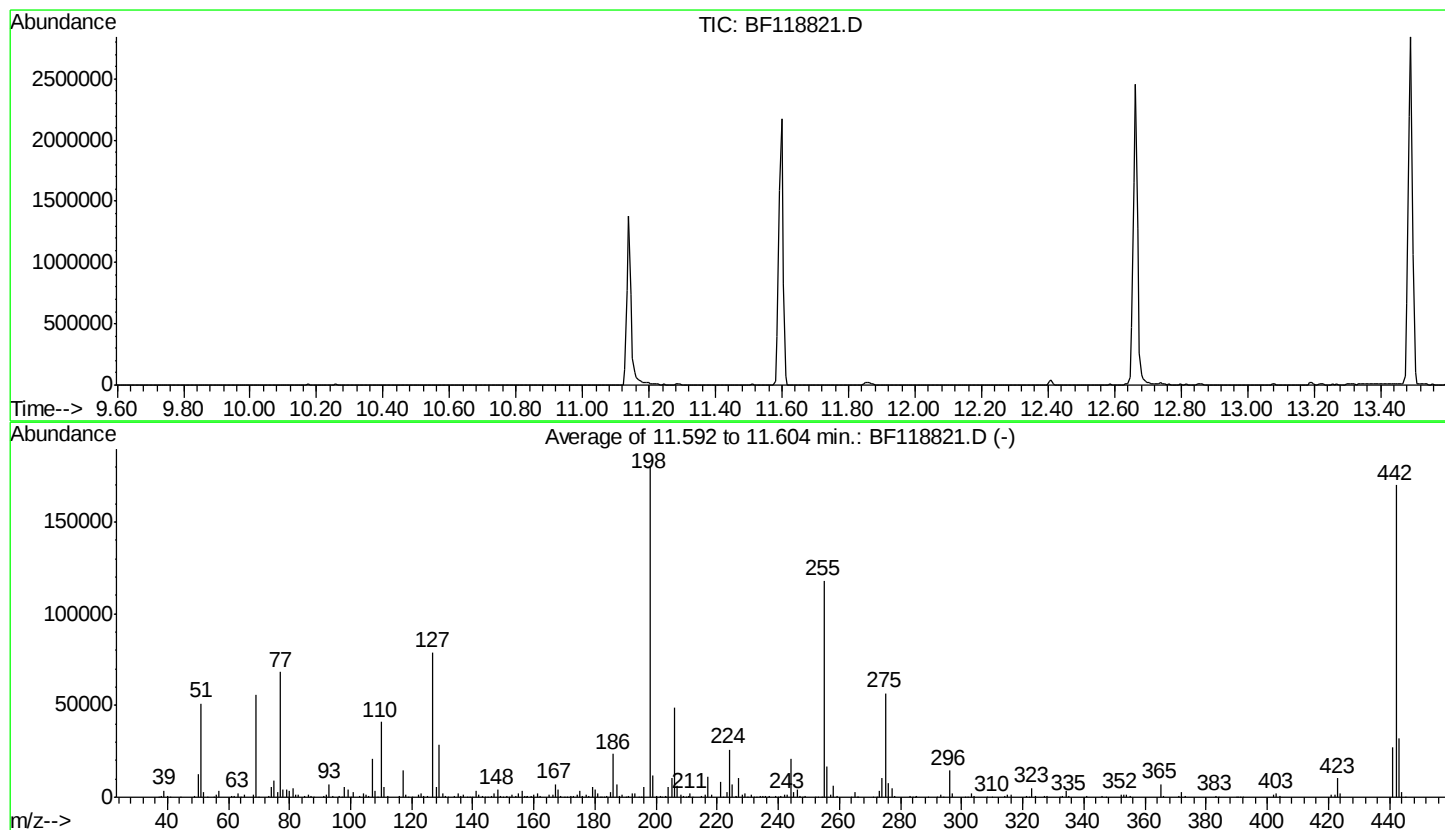

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	50944	PASS
68	69	0.00	2	1.9	1078	PASS
69	198	0.00	100	31.1	56106	PASS
70	69	0.00	2	0.4	201	PASS
127	198	10	80	43.6	78730	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	180666	PASS
199	198	5	9	6.6	11999	PASS
275	198	10	60	31.4	56714	PASS
365	198	1	100	3.9	7062	PASS
441	198	0.01	100	14.9	26994	PASS
442	198	50	100	94.0	169896	PASS
443	442	15	24	19.1	32376	PASS