

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020524\
 Data File : BF137273.D
 Acq On : 05 Feb 2024 12:41
 Operator : CG\JU
 Sample : P1340-01DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1DL

Quant Time: Feb 05 13:13:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 04:56:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-6.79
21) Naphthalene-d8	0.000	136	0	0.000	ng	-8.07
39) Acenaphthene-d10	0.000	164	0	0.000	ng	-9.83
64) Phenanthrene-d10	0.000	188	0	0.000	ng	-11.32
76) Chrysene-d12	0.000	240	0	0.000	ng	-13.97
86) Perylene-d12	0.000	264	0	0.000	ng	-15.46
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0	0.000	ng	
7) Phenol-d6	0.000	99	0	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
79) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020524\
Data File : BF137273.D
Acq On : 05 Feb 2024 12:41
Operator : CG\JU
Sample : P1340-01DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1DL

Quant Time: Feb 05 13:13:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

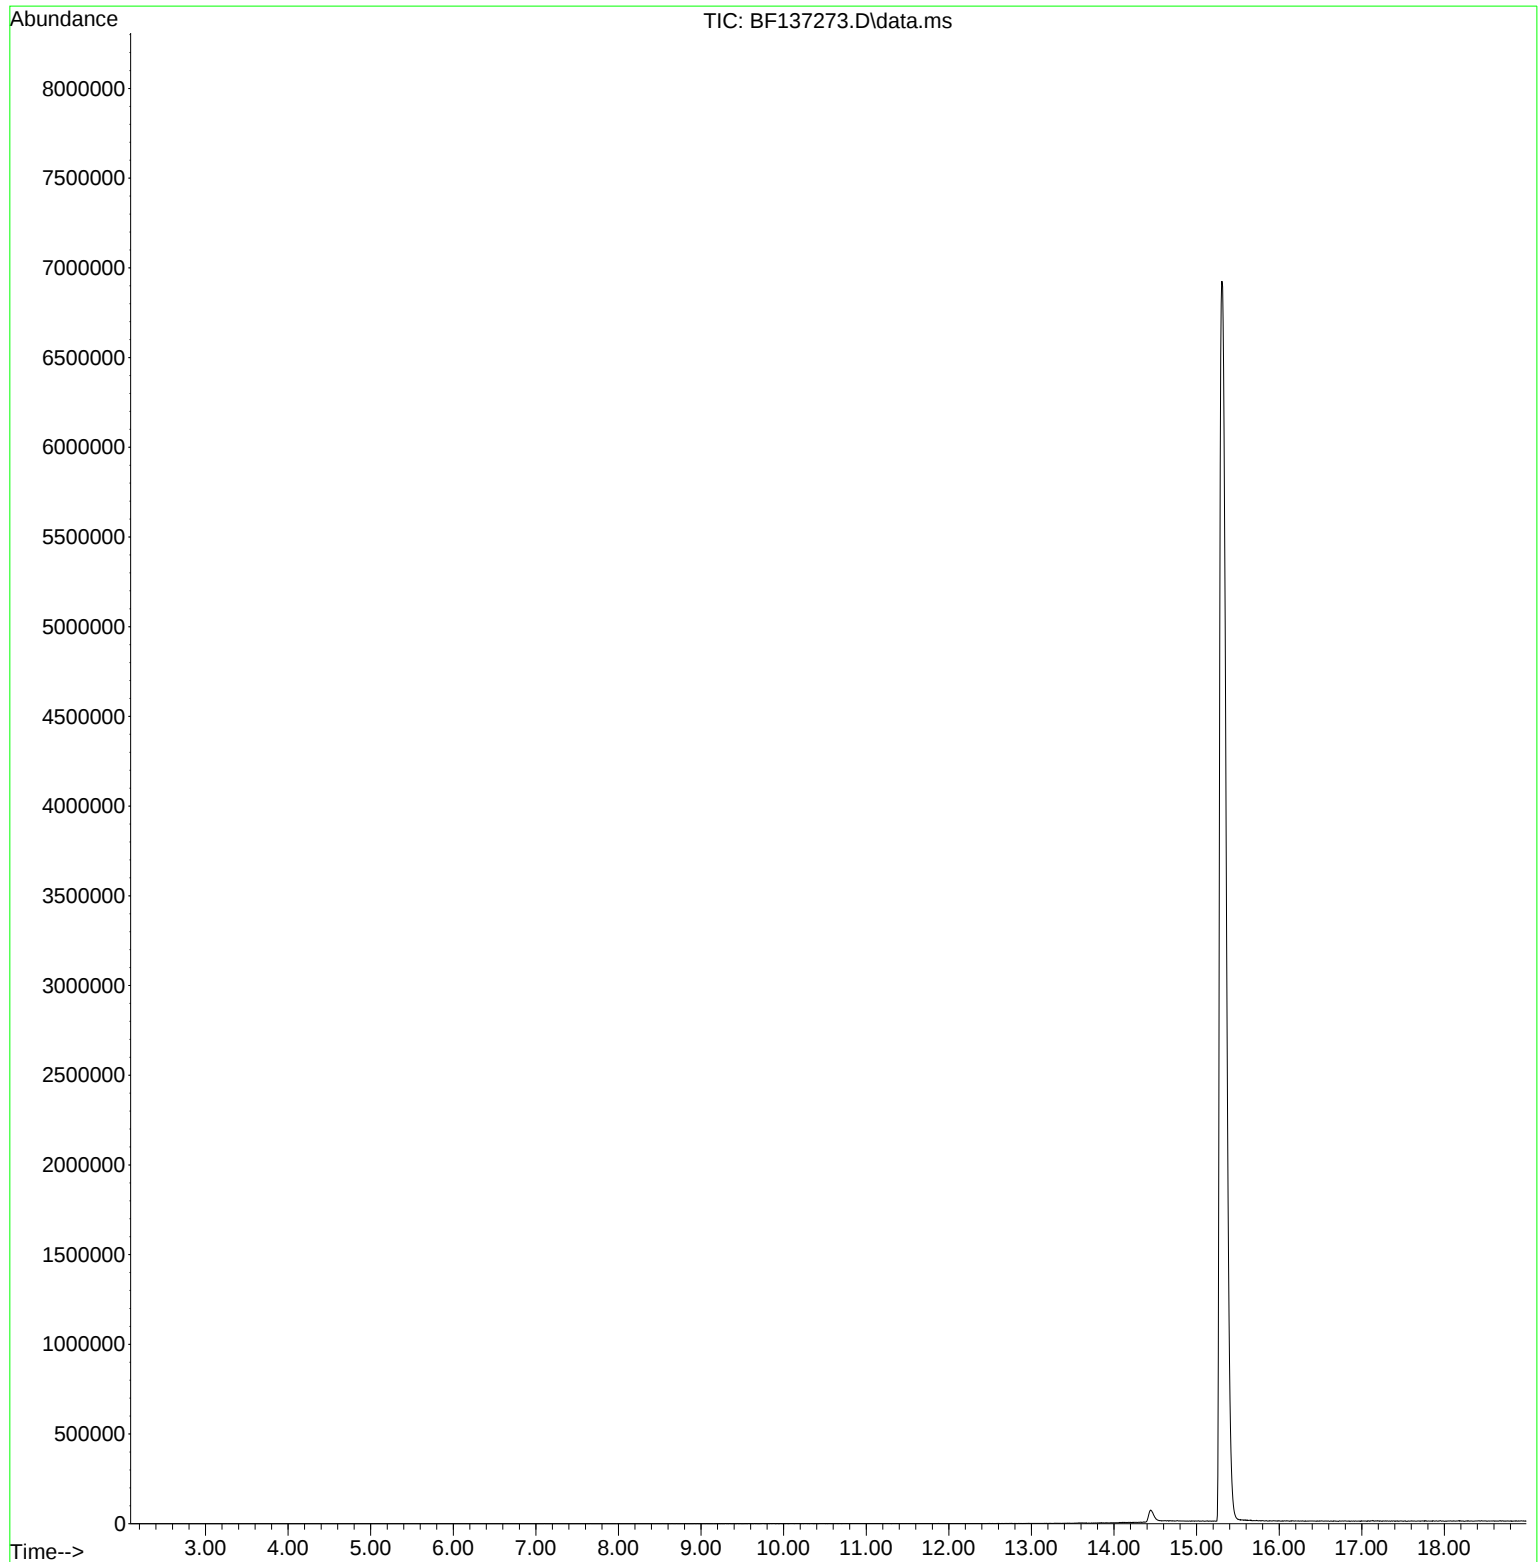

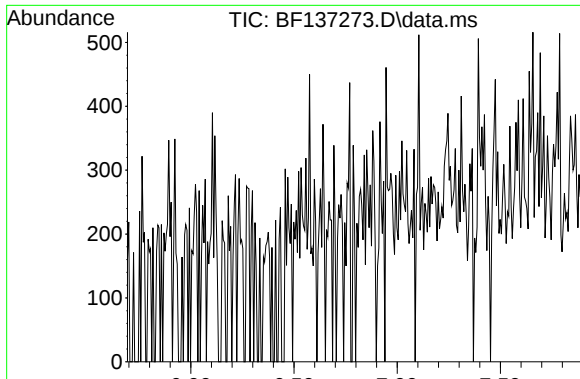



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ng
 Expected RT: 6.79 min

 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1DL

Tgt Ion: 152

Sig	Exp Ratio
152	100
150	162.3
115	73.1

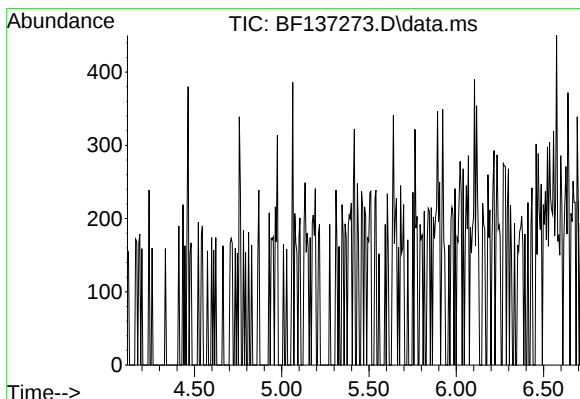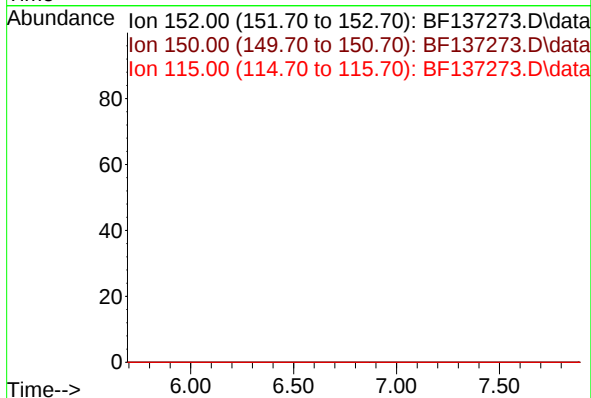



#5
 2-Fluorophenol
 Concen: 0.000 ng
 Expected RT: 5.42 min

 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Tgt Ion: 112

Sig	Exp Ratio
112	100
64	72.2
63	39.2

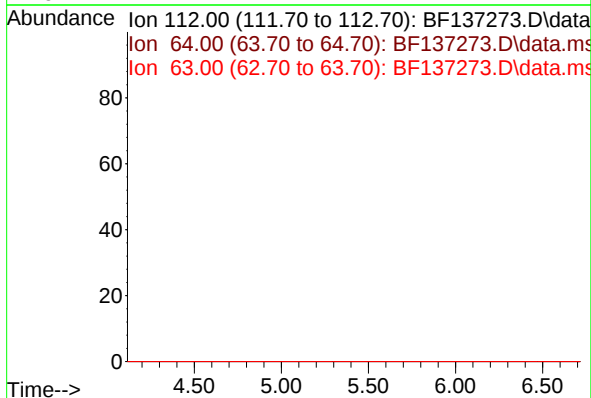


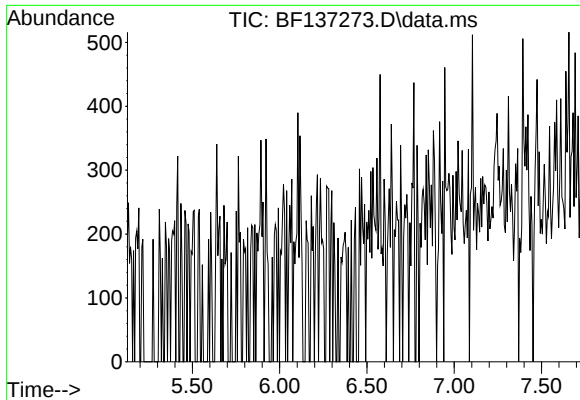


#7
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.43 min
 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1DL

Tgt Ion: 99


Sig	Exp Ratio
99	100
42	20.5
71	40.5

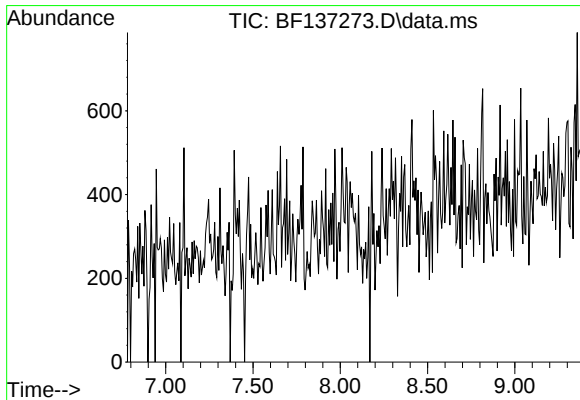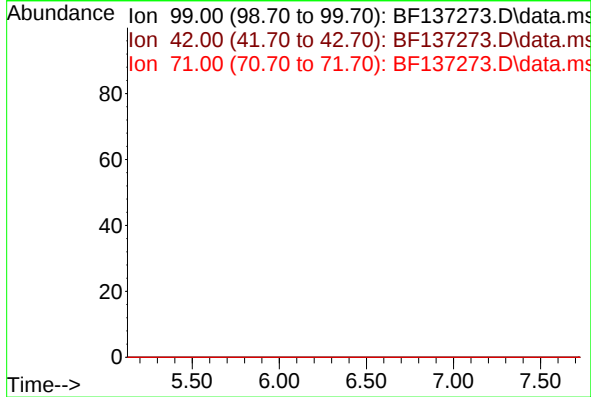


#21
 Naphthalene-d8
 Concen: 0.000 ng
 Expected RT: 8.07 min
 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Tgt Ion: 136

Sig	Exp Ratio
136	100
137	11.1
54	9.8
68	5.6

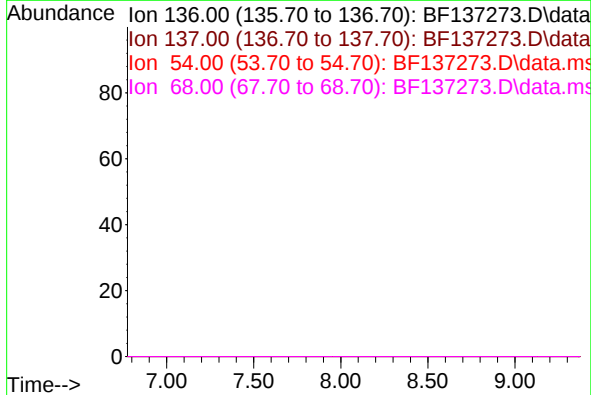


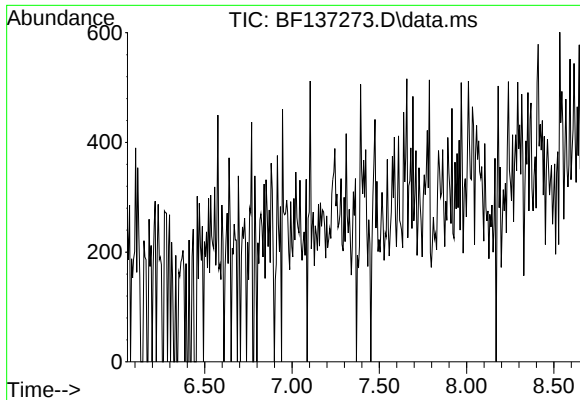


#23
Nitrobenzene-d5
Concen: 0.000 ng
Expected RT: 7.36 min

Lab File: BF137273.D
Acq: 05 Feb 2024 12:41

Instrument :
BNA_F
ClientSampleId :
COMP-1DL


Tgt Ion: 82
Sig Exp Ratio
82 100
128 36.4
54 56.3

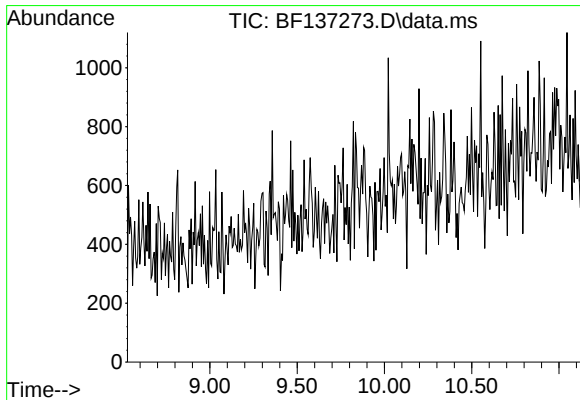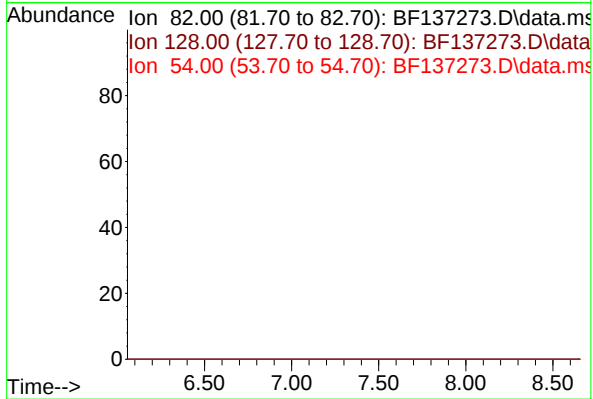


#39
Acenaphthene-d10
Concen: 0.000 ng
Expected RT: 9.83 min

Lab File: BF137273.D
Acq: 05 Feb 2024 12:41

Tgt Ion: 164
Sig Exp Ratio
164 100
162 97.9
160 44.3

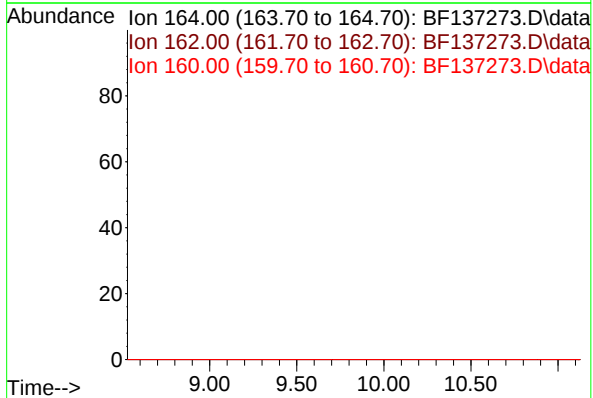


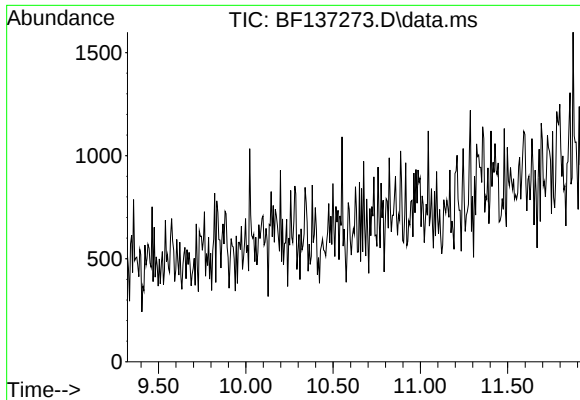


#42
 2,4,6-Tribromophenol
 Concen: 0.000 ng
 Expected RT: 10.62 min
 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1DL

Tgt Ion: 330


Sig	Exp Ratio
330	100
332	96.6
141	31.5

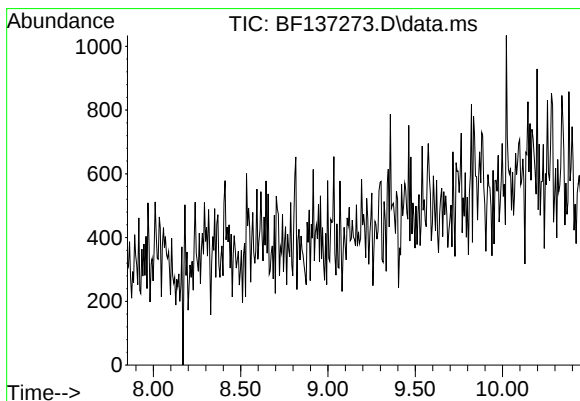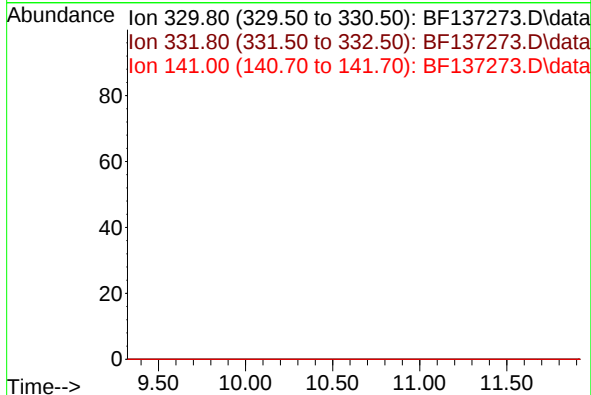


#45
 2-Fluorobiphenyl
 Concen: 0.000 ng
 Expected RT: 9.15 min
 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Tgt Ion: 172

Sig	Exp Ratio
172	100
171	35.4
170	23.9

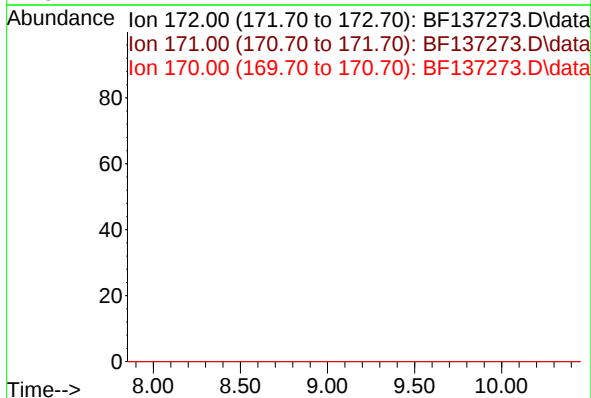


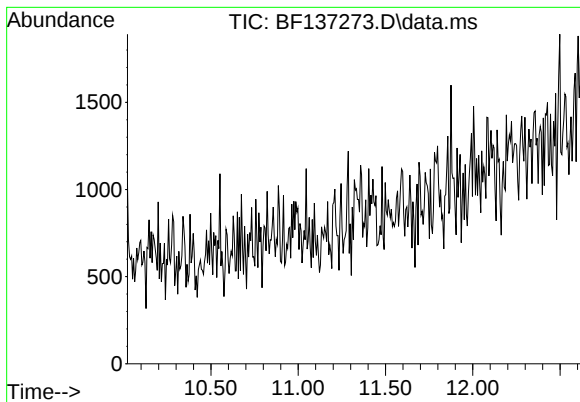


#64
 Phenanthrene-d10
 Concen: 0.000 ng
 Expected RT: 11.32 min
 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1DL

Tgt Ion: 188


Sig	Exp Ratio
188	100
94	8.7
80	11.0

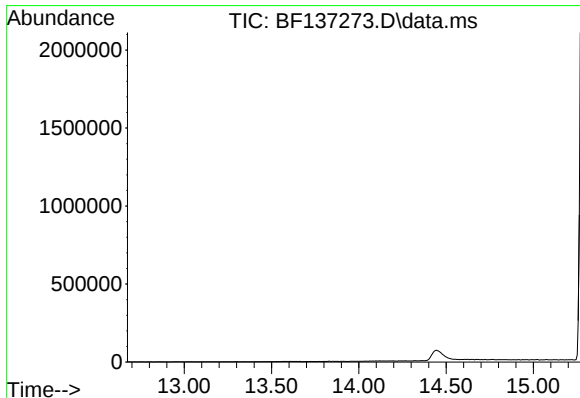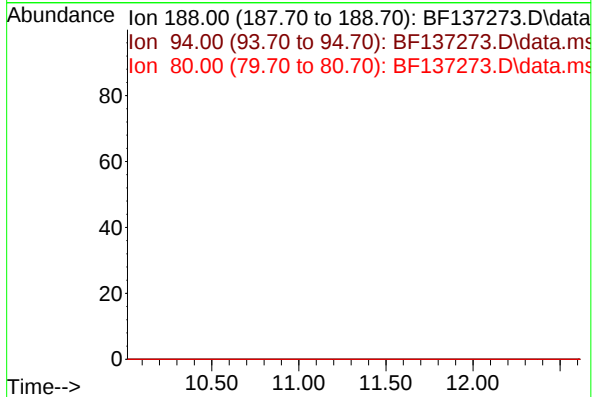


#76
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 13.97 min
 Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Tgt Ion: 240

Sig	Exp Ratio
240	100
120	7.9
236	25.4

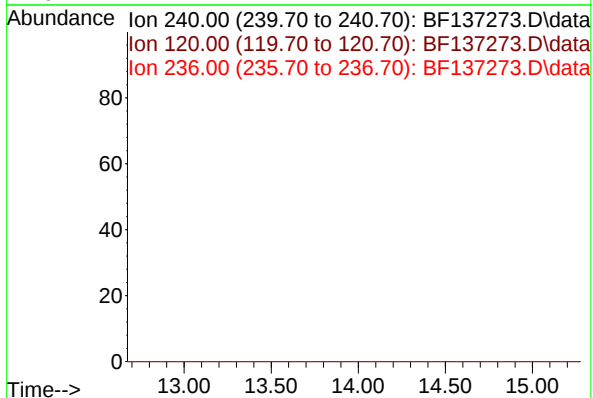


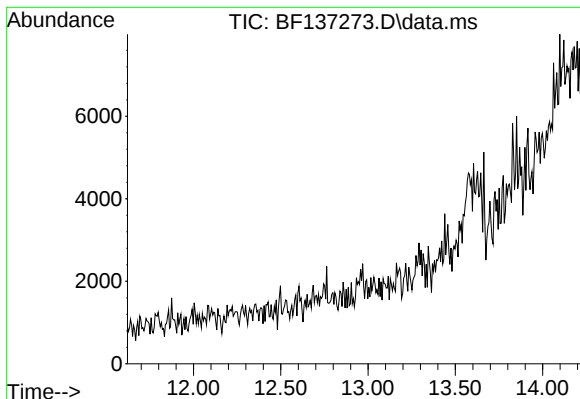


#79
 Terphenyl-d14
 Concen: 0.000 ng
 Expected RT: 12.92 min

Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1DL

Tgt Ion: 244
 Sig Exp Ratio
 244 100
 212 6.9
 122 7.8

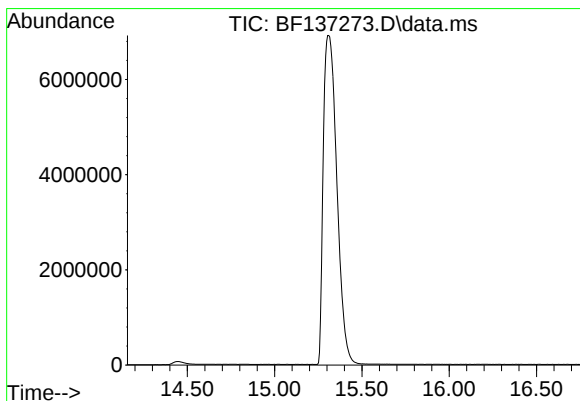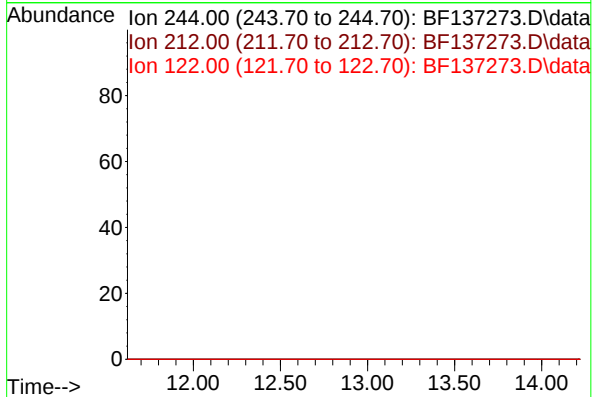

#86
 Perylene-d12
 Concen: 0.000 ng
 Expected RT: 15.46 min

Lab File: BF137273.D
 Acq: 05 Feb 2024 12:41

Tgt Ion: 264
 Sig Exp Ratio
 264 100
 260 22.8
 265 20.2

