


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020524\
Data File : BF137268.D
Acq On : 05 Feb 2024 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 31 04:56:22 2024

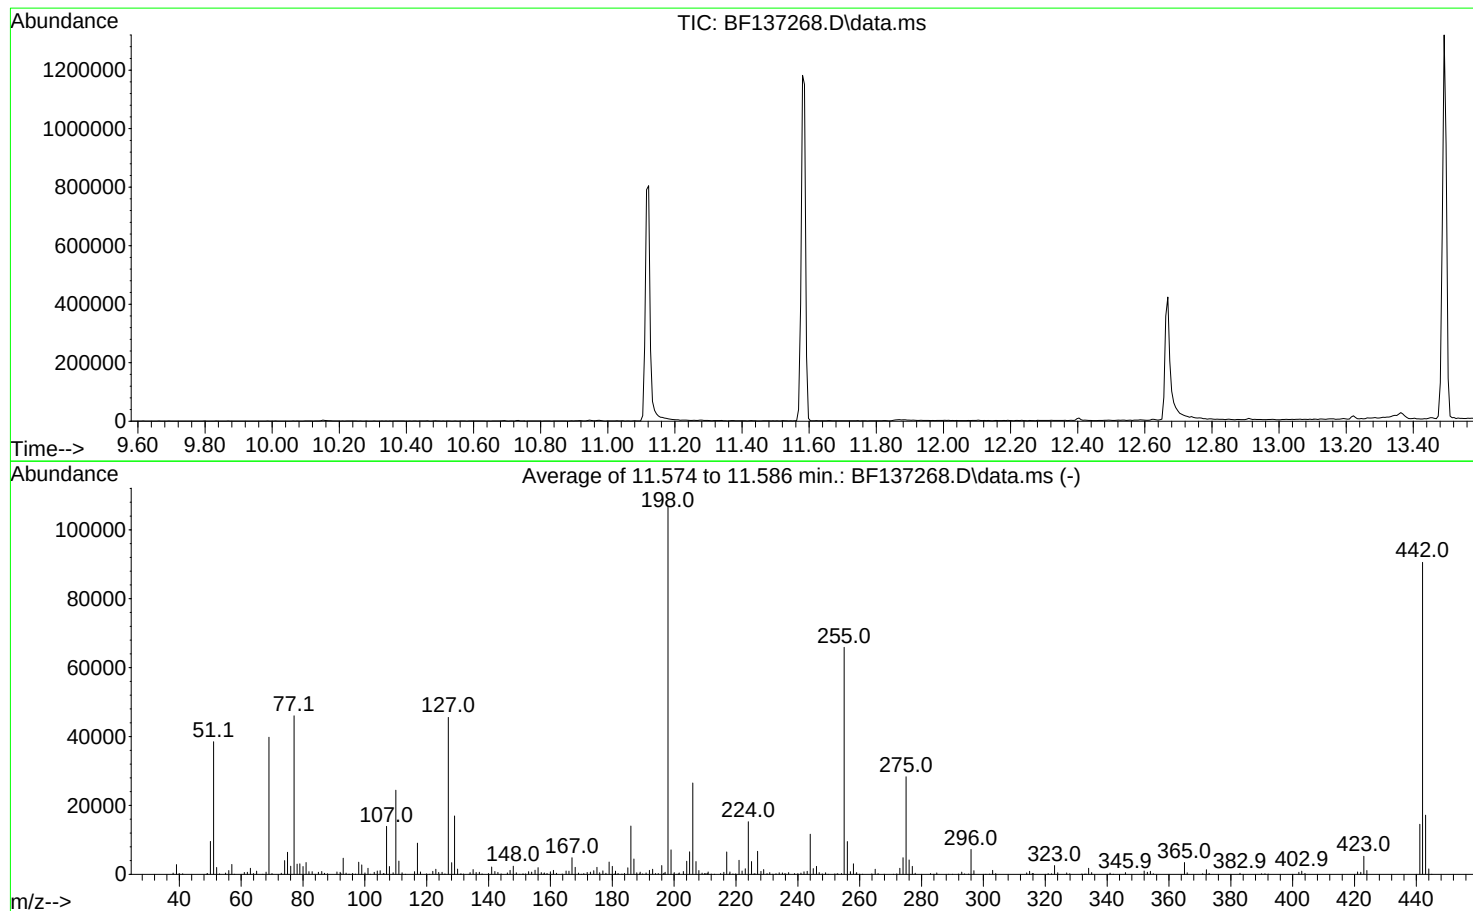




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	38507	PASS
68	69	0.00	2	1.6	653	PASS
69	198	0.00	100	37.3	39797	PASS
70	69	0.00	2	0.6	219	PASS
127	198	10	80	42.7	45579	PASS
197	198	0.00	2	0.6	617	PASS
198	198	100	100	100.0	106768	PASS
199	198	5	9	6.6	7090	PASS
275	198	10	60	26.5	28342	PASS
365	198	1	100	3.2	3423	PASS
441	198	0.01	100	13.6	14522	PASS
442	442	50	100	100.0	90573	PASS
443	442	15	24	19.0	17185	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020524\
Data File : BF137268.D
Acq On : 05 Feb 2024 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 05 11:17:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

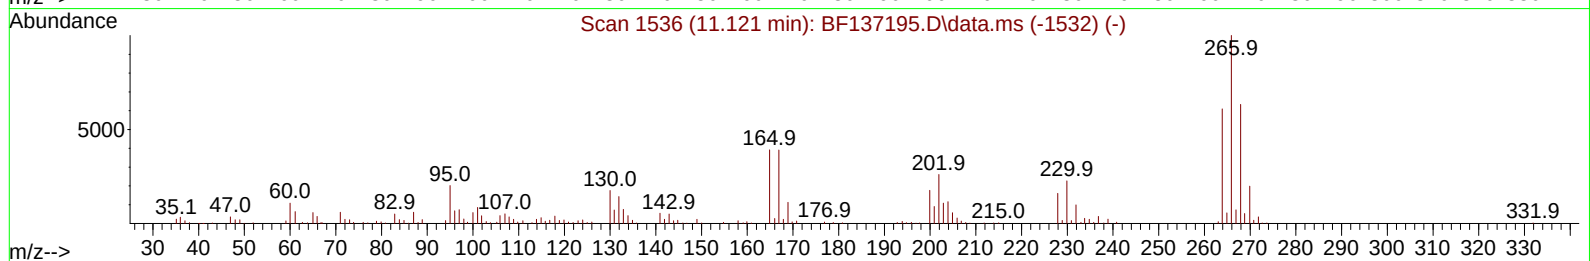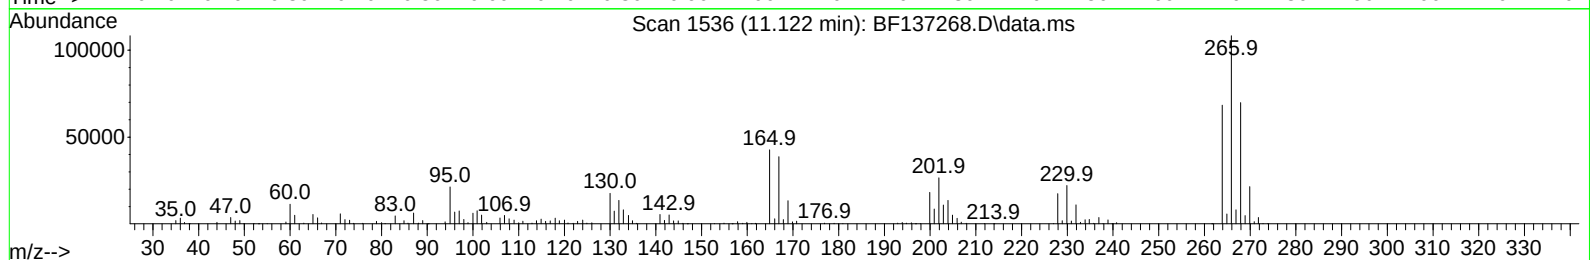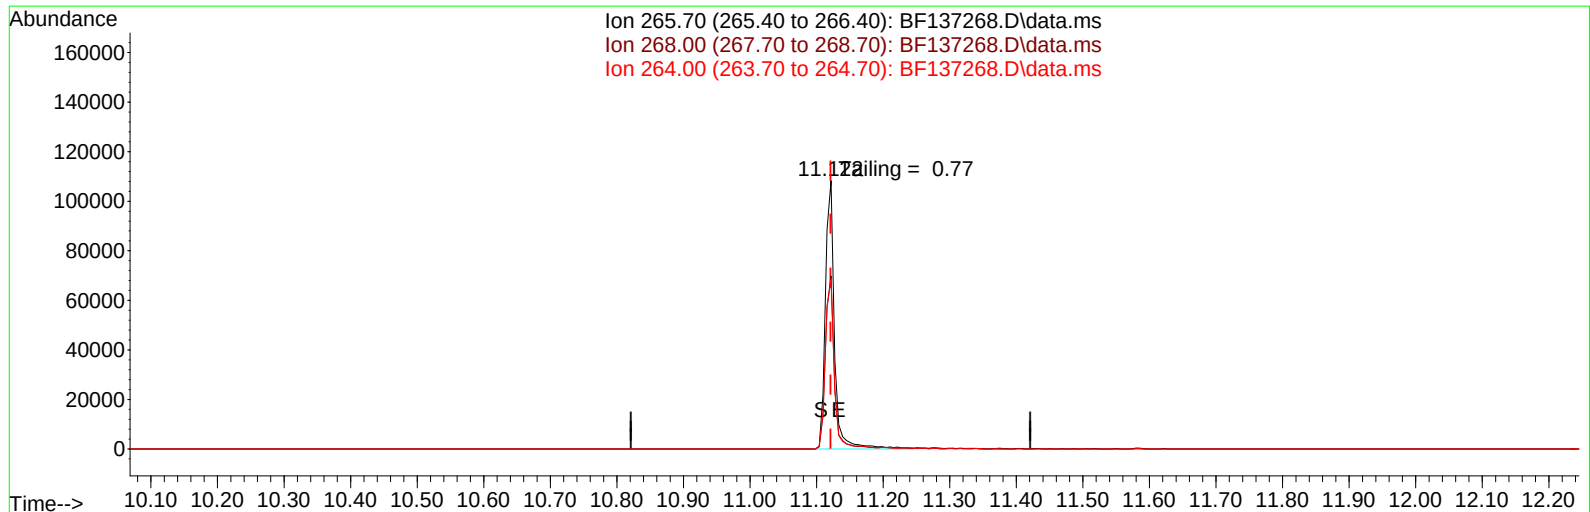

TIC: BF137268.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.001) 239744.94 ng m

response 102965

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.48
264.00	61.00	63.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/5/2024	BNA_F	<u>BF137268.D</u>
Compound Name	Response	Retention Time
DDT	220927	13.492
DDD	3168	13.221
DDE	193	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3361	224288	1.50

Instrument :
BNA_F
ClientSampleId :
DFTPP