
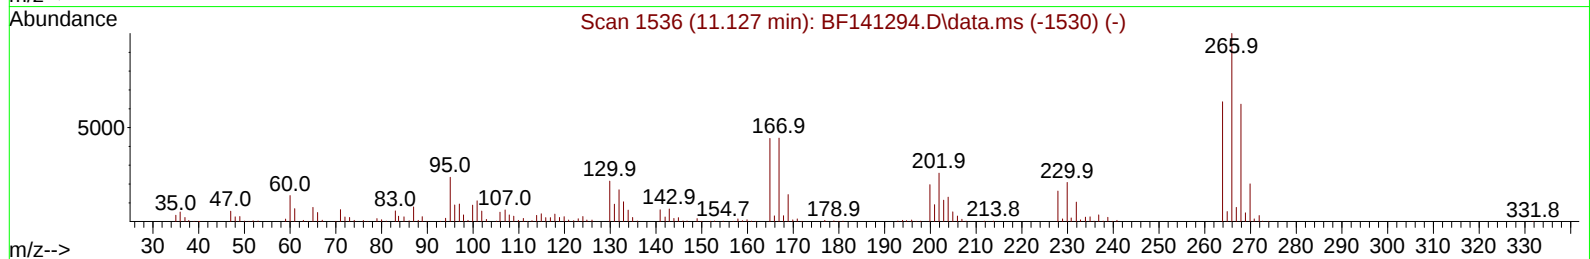
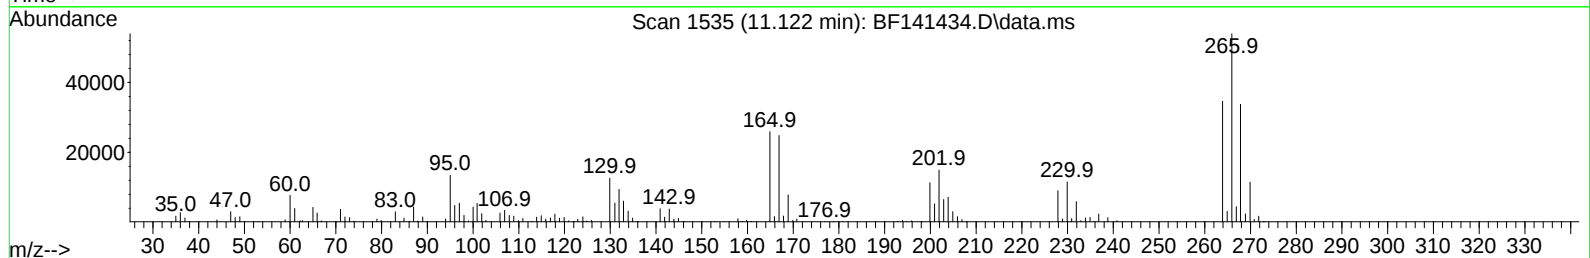


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141434.D
Acq On : 05 Feb 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 10:46:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

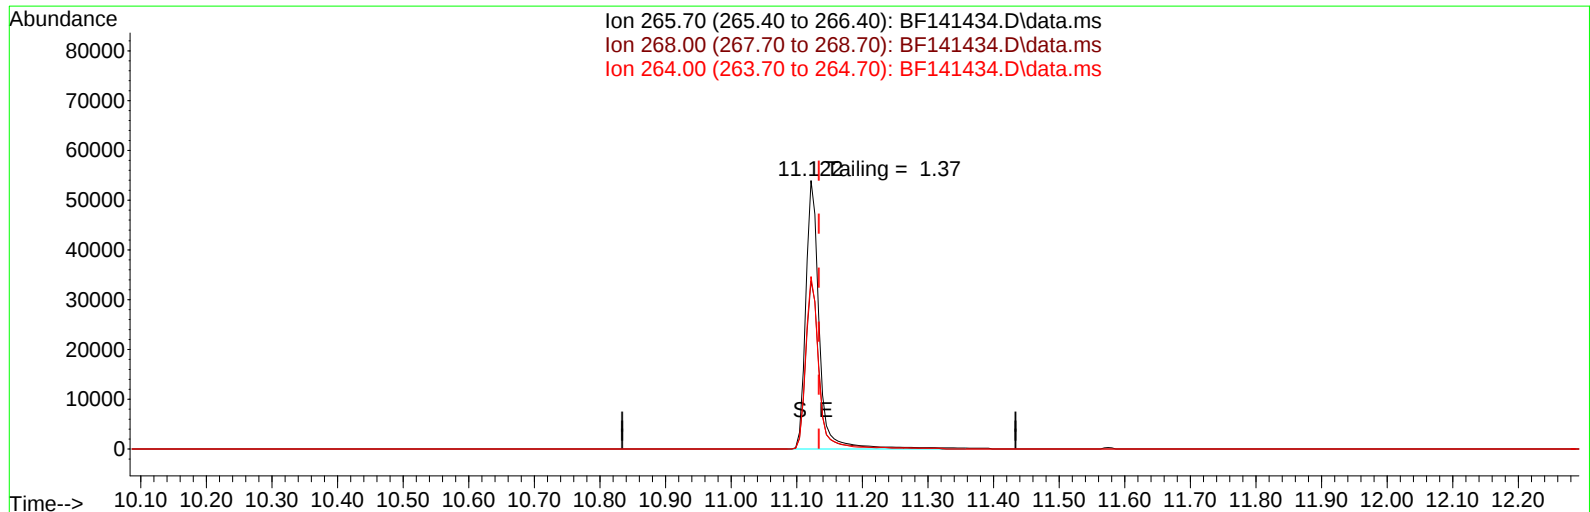

TIC: BF141434.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.012) 27136.66 ng

response 77371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.57
264.00	63.70	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141434.D
Acq On : 05 Feb 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 10:46:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

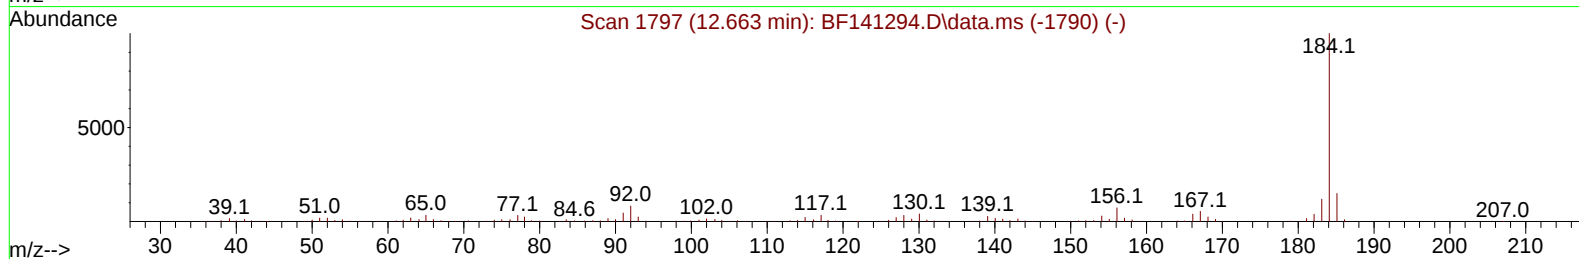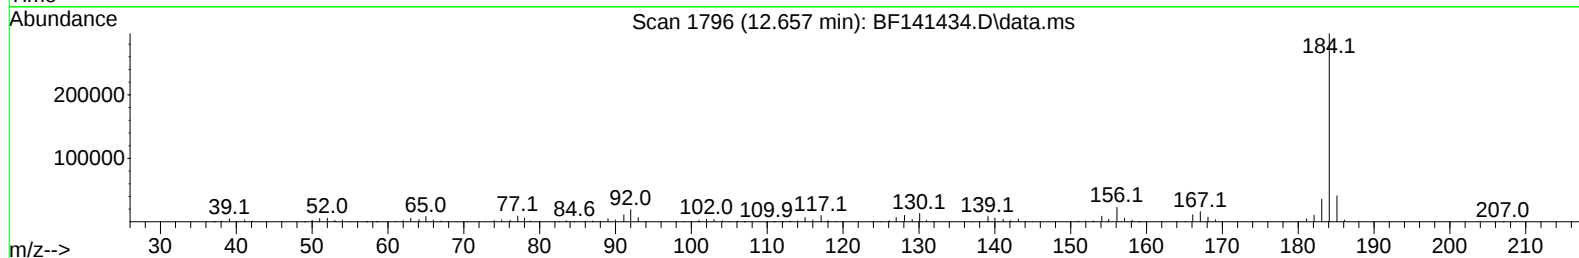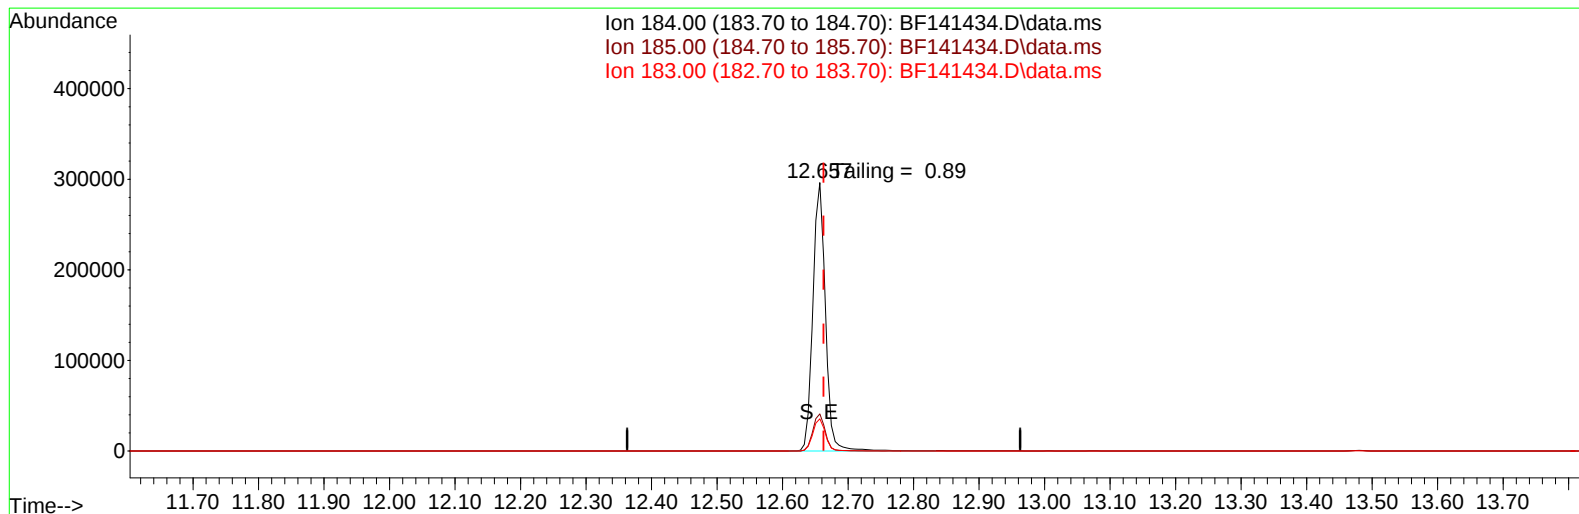

TIC: BF141434.D\data.ms

(77) Benzidine

12.657min (-0.006) 0.00 ng

response 393319

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.83
183.00	11.90	12.02
0.00	0.00	0.00