


Data Path : Z:\HPCHEM1\BNA F\Data\BF020615\
Data File : BF077201.D
Acq On : 6 Feb 2015 12:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 30 22:48:24 2015

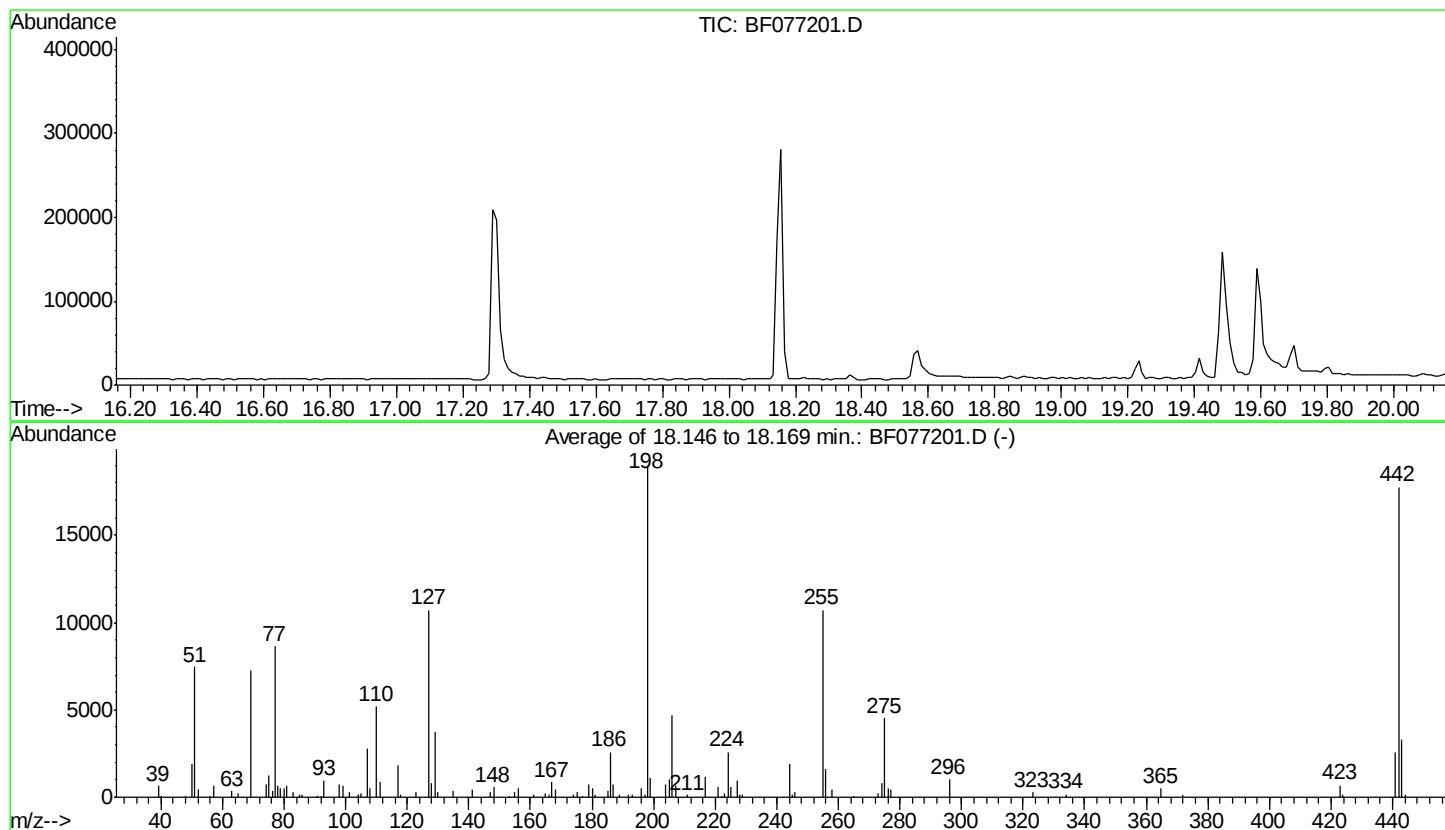

AutoFind: Scans 1510, 1511, 1512; Background Corrected with Scan 1506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	7461	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.2	7257	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.4	10709	PASS
197	198	0.00	2	0.6	123	PASS
198	198	100	100	100.0	18987	PASS
199	198	5	9	5.8	1109	PASS
275	198	10	60	23.8	4510	PASS
365	198	1	100	2.7	507	PASS
441	442	0.01	24	14.5	2574	PASS
442	198	50	100	93.5	17754	PASS
443	442	15	24	18.5	3292	PASS