

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
 Data File : BF077206.D
 Acq On : 6 Feb 2015 17:27
 Operator : TP/IZ
 Sample : G1238-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.001	9	10	30	rVB3	83895	193178	13.41%	2.080%
2	1.298	35	36	41	rVV	94658	164384	11.41%	1.770%
3	1.367	41	42	59	rVB	757819	1440480	100.00%	15.512%
4	2.635	148	153	159	rBV	304751	647355	44.94%	6.971%
5	3.687	243	245	255	rBV	22749	65095	4.52%	0.701%
6	4.658	328	330	344	rBV	130143	324257	22.51%	3.492%
7	7.059	537	540	544	rBV	75855	157972	10.97%	1.701%
8	7.127	544	546	556	rVB	379506	720414	50.01%	7.758%
9	7.642	589	591	600	rBV	96313	170072	11.81%	1.831%
10	7.962	616	619	627	rBV	409770	667564	46.34%	7.189%
11	8.945	702	705	719	rVB	284309	515845	35.81%	5.555%
12	10.556	843	846	851	rBV	139042	232576	16.15%	2.505%
13	13.208	1074	1078	1081	rBV	704778	1058046	73.45%	11.394%
14	14.671	1203	1206	1212	rBV	155502	259019	17.98%	2.789%
15	16.408	1356	1358	1365	rVB	409823	609840	42.34%	6.567%
16	17.540	1454	1457	1461	rBV	235695	275153	19.10%	2.963%
17	19.791	1651	1654	1656	rVB	810097	1133854	78.71%	12.210%
18	21.049	1760	1764	1769	rBV	265931	367410	25.51%	3.957%
19	22.695	1905	1908	1913	rVB	164160	258193	17.92%	2.780%
20	23.312	1957	1962	1964	rBV4	8397	25381	1.76%	0.273%


Sum of corrected areas: 9286088

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077206.D
Acq On : 6 Feb 2015 17:27
Operator : TP/IZ
Sample : G1238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

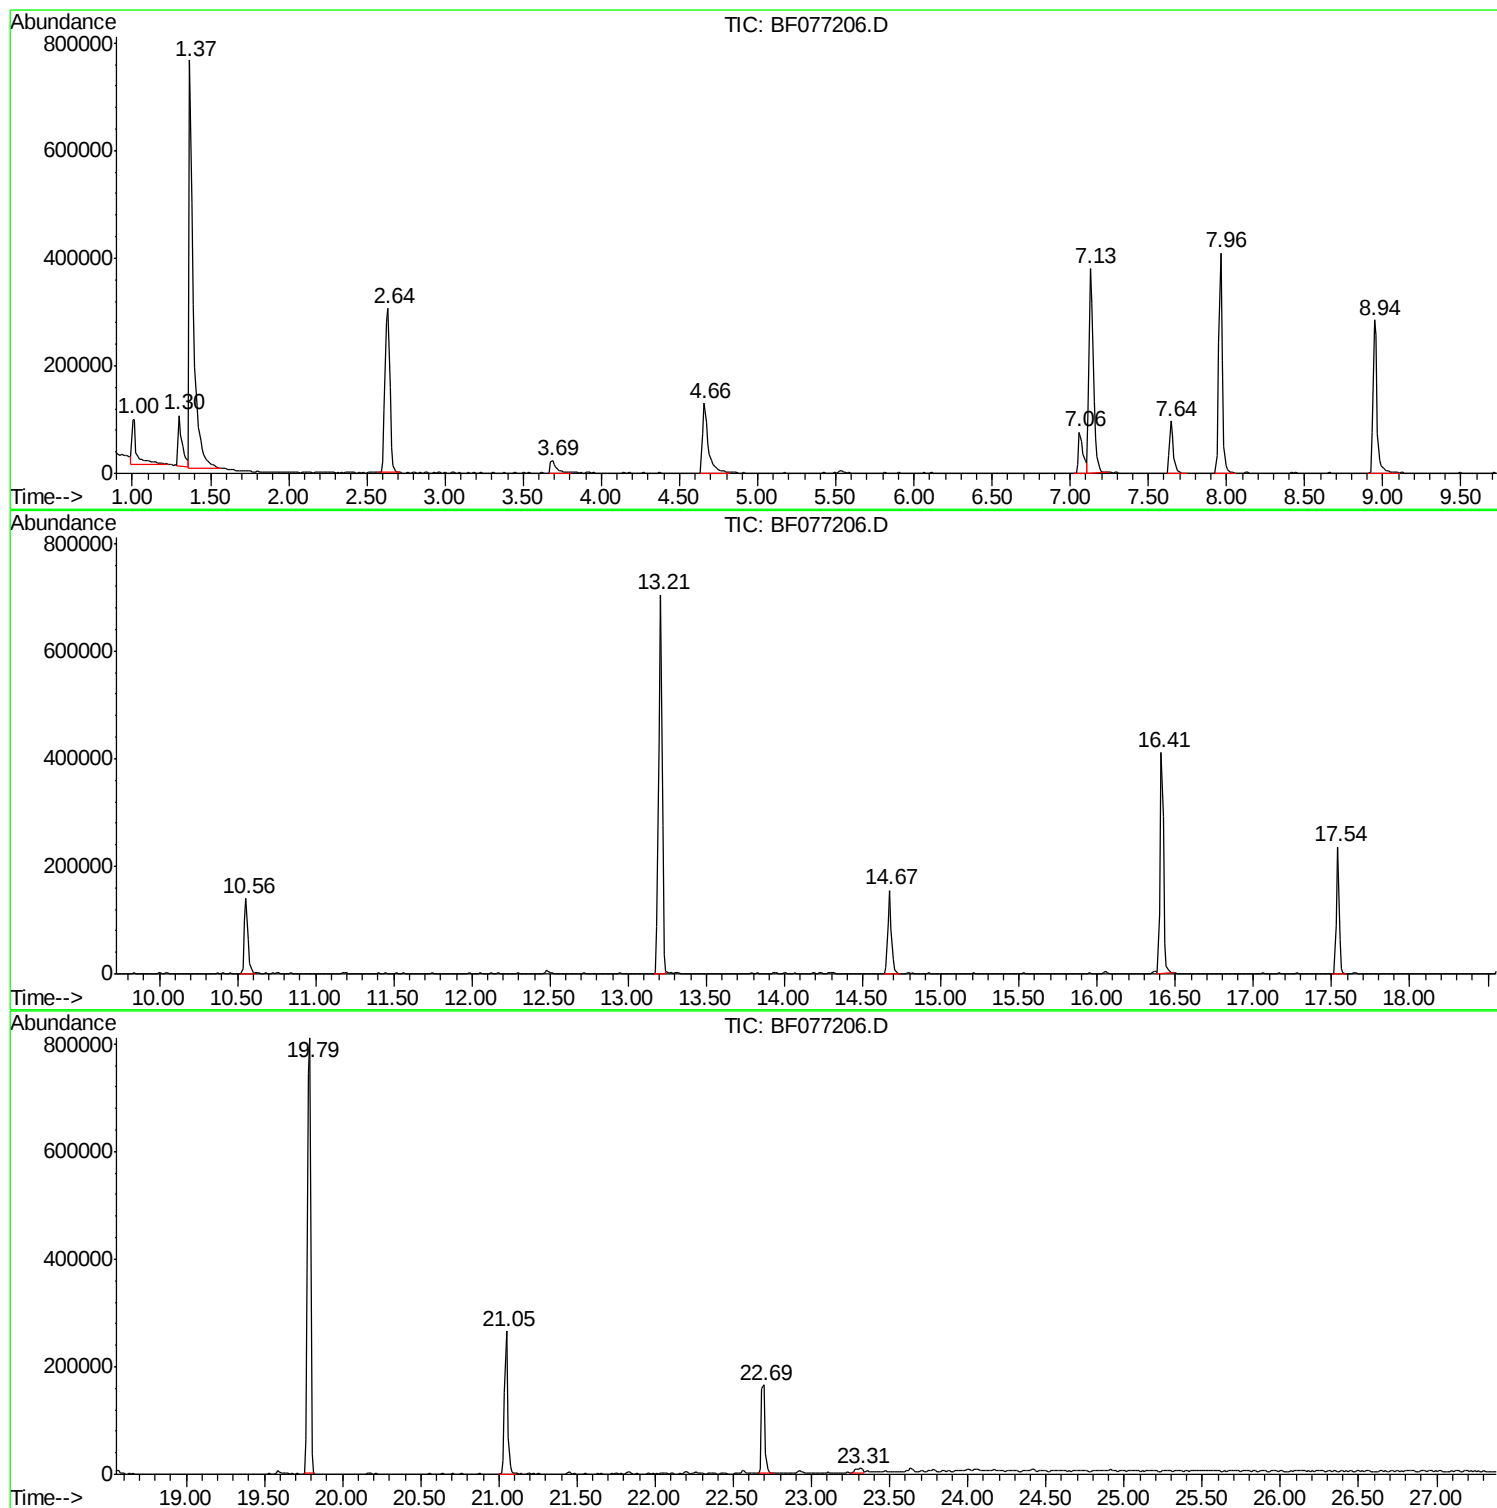

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077206.D
Acq On : 6 Feb 2015 17:27
Operator : TP/IZ
Sample : G1238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown3.69 Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.69	7.65 ng	65095	1,4-Dichlorobenzene-d4	7.64

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	36
2		Acetone	58	C3H6O	000067-64-1	9
3		2-Nonanone	142	C9H18O	000821-55-6	9
4		3-Octanol	130	C8H18O	000589-98-0	9
5		Hexane, 4-ethyl-2,2-dimethyl-	142	C10H22	052896-99-8	9

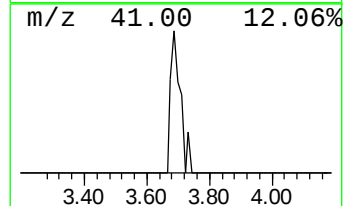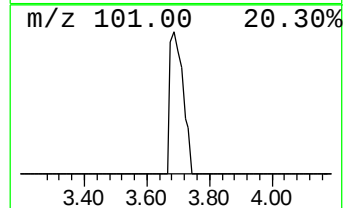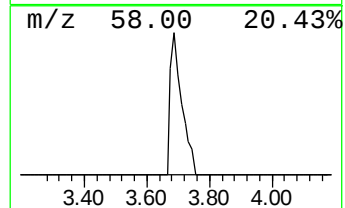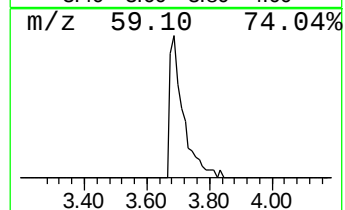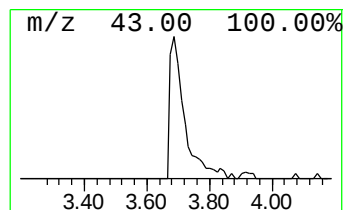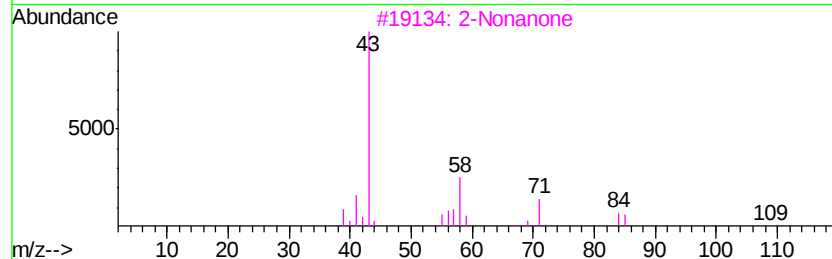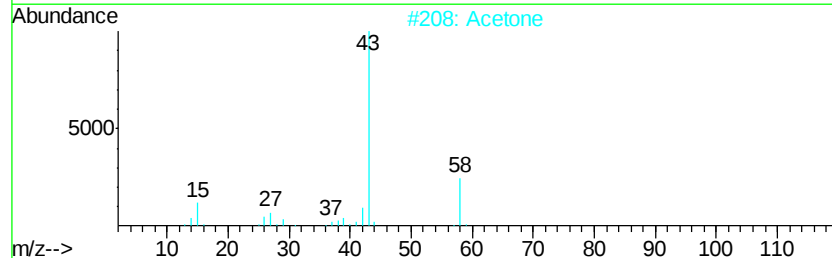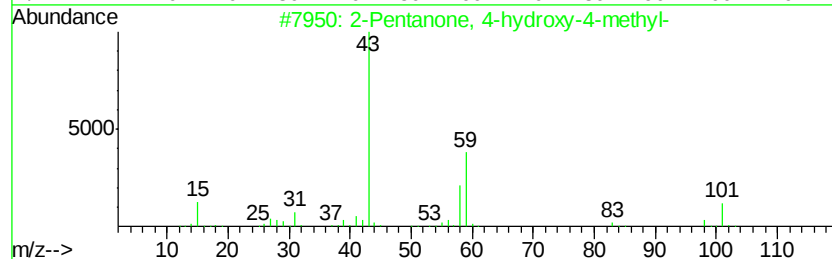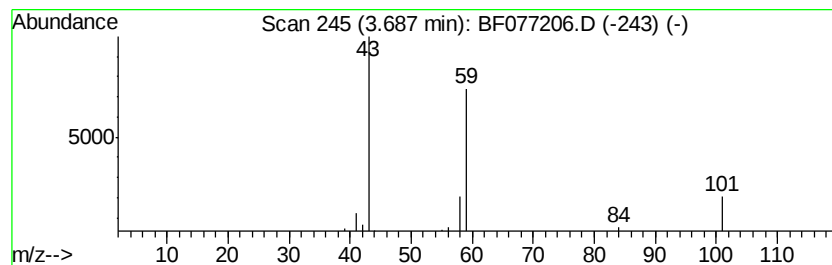

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF0720615\
Data File : BF077206.D
Acq On : 6 Feb 2015 17:27
Operator : TP/IZ
Sample : G1238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 unknown7.13 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.13	84.72 ng	720414	1,4-Dichlorobenzene-d4	7.64

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	10
5		1,2,3-Trifluorobenzene	132	C6H3F3	001489-53-8	9

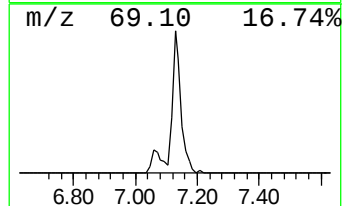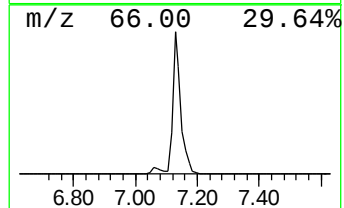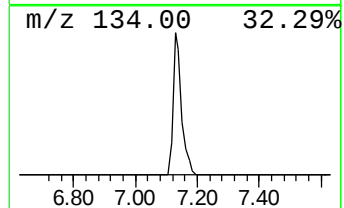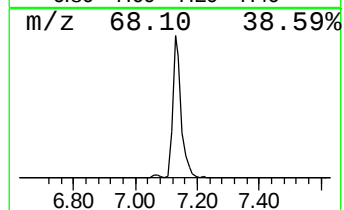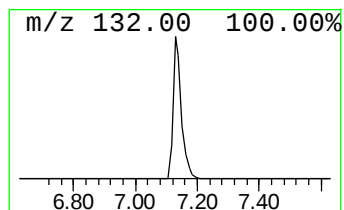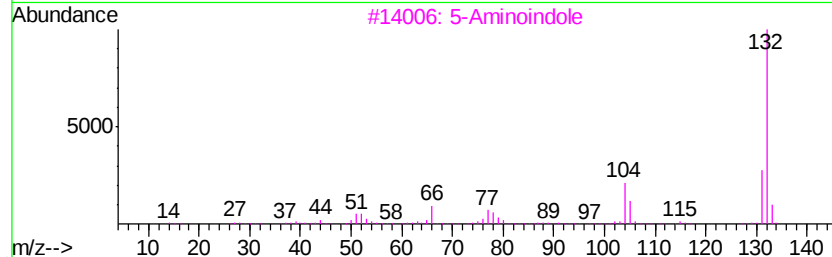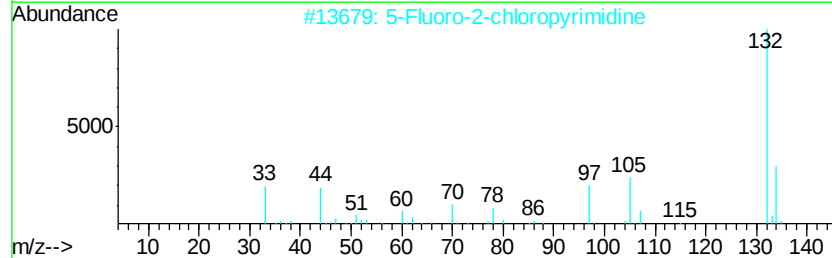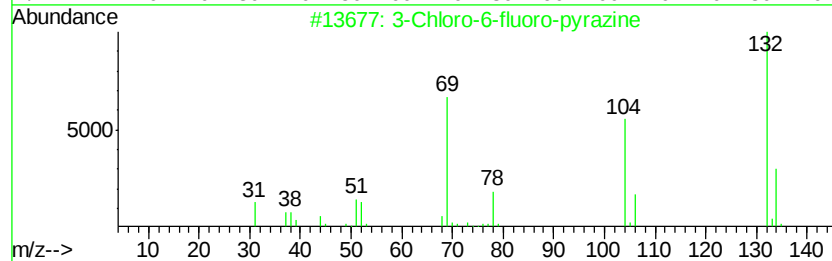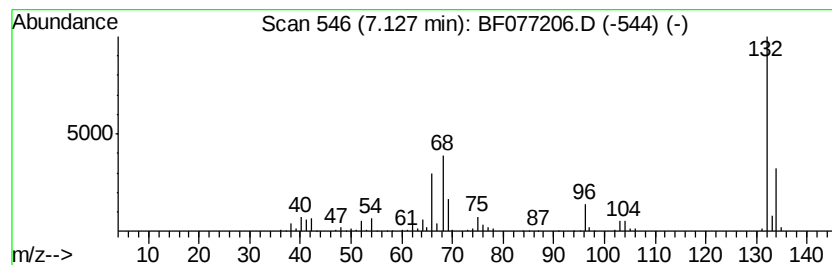

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077206.D
Acq On : 6 Feb 2015 17:27
Operator : TP/IZ
Sample : G1238-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.69	3.69	7.7	ng	65095	1	7.64	170072	20.0
unknown7.13	7.13	84.7	ng	720414	1	7.64	170072	20.0