

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
 Data File : BF077209.D
 Acq On : 6 Feb 2015 19:11
 Operator : TP/IZ
 Sample : PB81634BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81634BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	35	36	41	rBV	11776	27745	2.21%	0.384%
2	1.367	41	42	51	rVB	33084	71108	5.67%	0.983%
3	3.687	242	245	258	rBV	69861	191558	15.26%	2.648%
4	4.659	327	330	345	rBV	233298	545854	43.49%	7.546%
5	7.048	537	539	544	rBV	278770	497289	39.62%	6.875%
6	7.128	544	546	556	rVB	336661	638784	50.89%	8.831%
7	7.642	589	591	600	rBV	89612	159046	12.67%	2.199%
8	7.962	616	619	630	rVB	407637	674545	53.74%	9.325%
9	8.945	703	705	719	rBV	277942	515363	41.06%	7.125%
10	10.556	843	846	851	rBV	127519	215833	17.20%	2.984%
11	13.208	1074	1078	1088	rBV	663904	1050395	83.68%	14.521%
12	14.671	1203	1206	1215	rBB2	142181	241954	19.28%	3.345%
13	16.408	1356	1358	1371	rVB	251219	381284	30.38%	5.271%
14	17.540	1455	1457	1463	rBV	211888	256634	20.45%	3.548%
15	19.792	1651	1654	1656	rBV	950224	1255183	100.00%	17.353%
16	21.049	1762	1764	1772	rBB	233911	266826	21.26%	3.689%
17	22.695	1905	1908	1915	rBV	194320	244006	19.44%	3.373%


Sum of corrected areas: 7233407

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
Data File : BF077209.D
Acq On : 6 Feb 2015 19:11
Operator : TP/IZ
Sample : PB81634BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81634BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

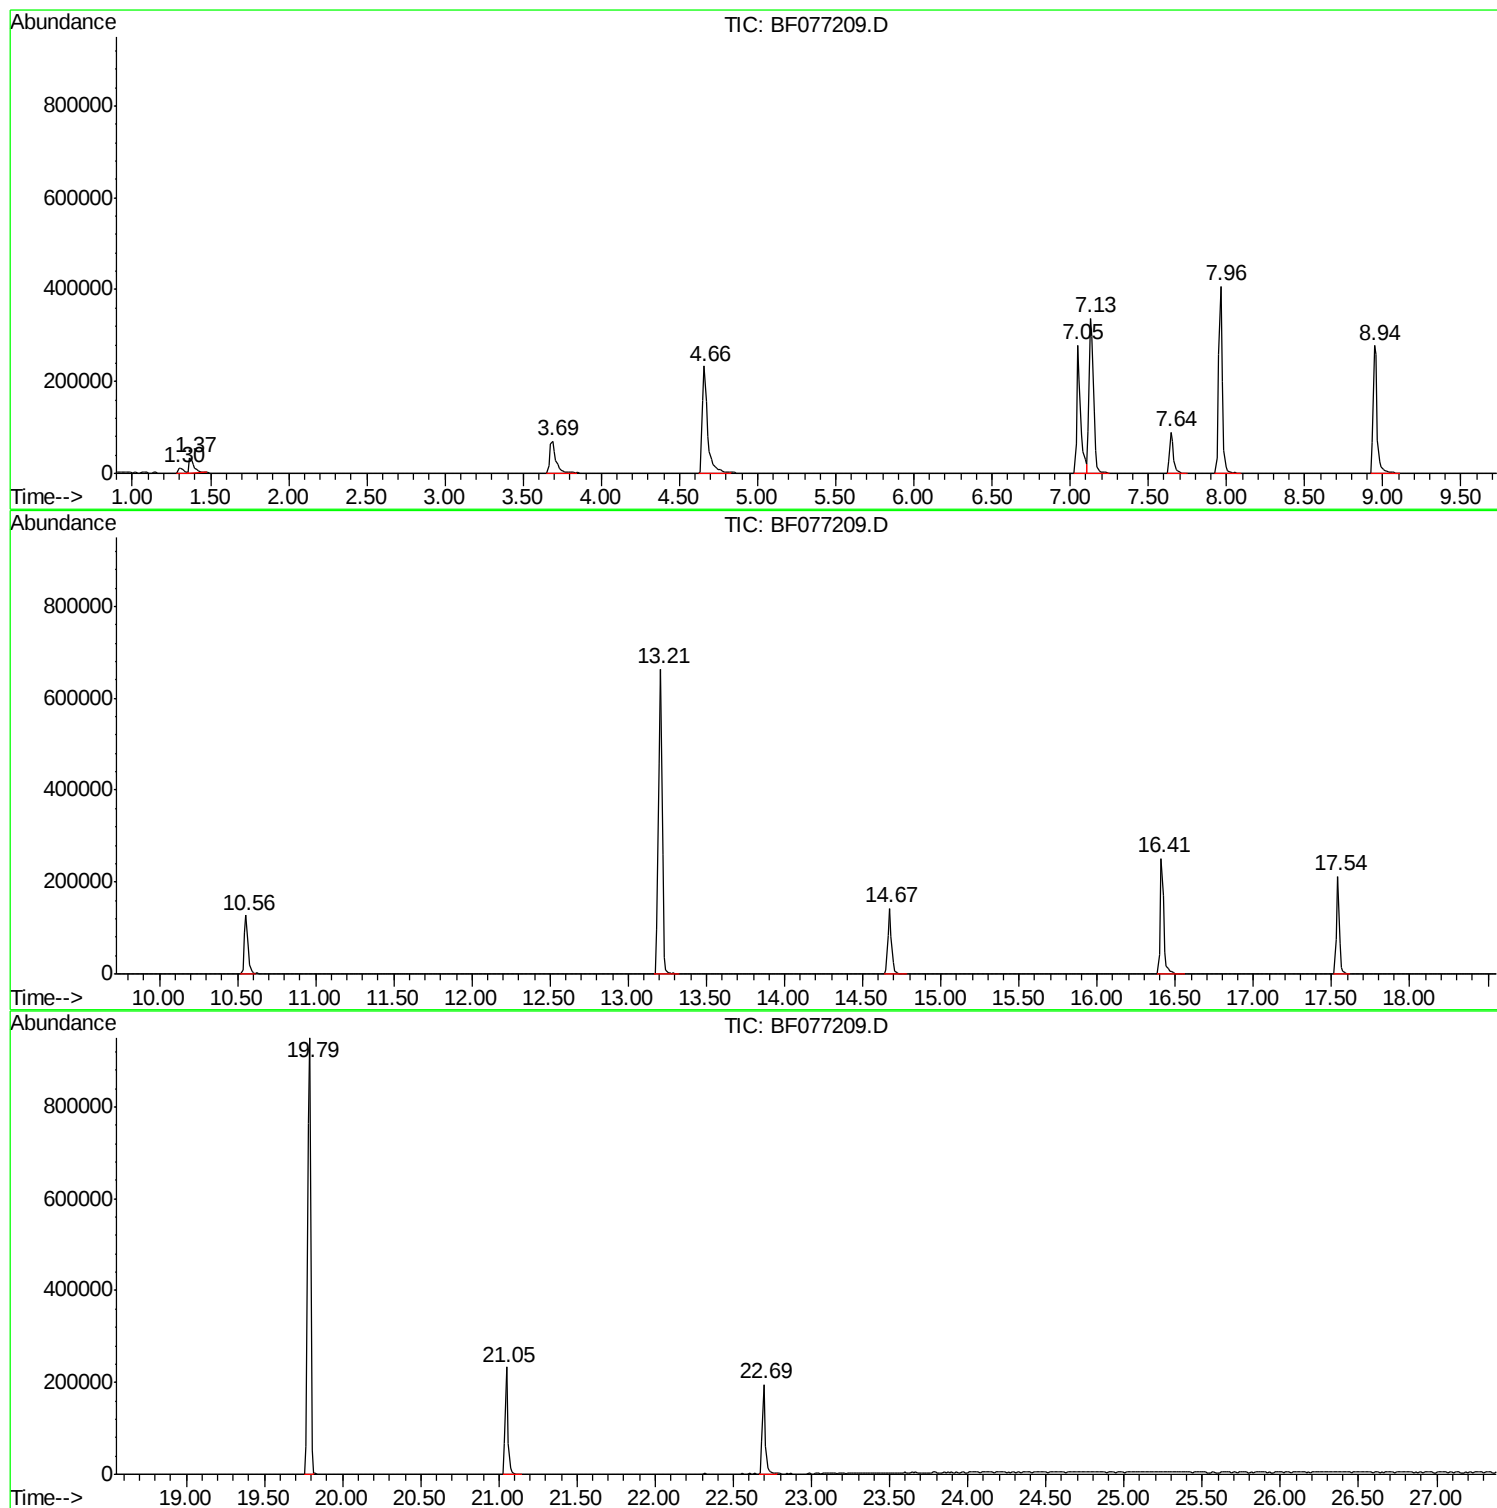

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
Data File : BF077209.D
Acq On : 6 Feb 2015 19:11
Operator : TP/IZ
Sample : PB81634BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81634BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
Data File : BF077209.D
Acq On : 6 Feb 2015 19:11
Operator : TP/IZ
Sample : PB81634BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81634BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc