

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
 Data File : BF077218.D
 Acq On : 7 Feb 2015 00:22
 Operator : TP/IZ
 Sample : G1251-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EXCAVATION-WATER-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	41	42	50	rVV	50548	104685	8.38%	1.499%
2	3.676	242	244	253	rBV	25353	70059	5.61%	1.003%
3	4.670	328	331	342	rBV	73932	191618	15.34%	2.744%
4	7.070	539	541	544	rBV	38109	80915	6.48%	1.159%
5	7.127	544	546	557	rVB	252812	545950	43.72%	7.817%
6	7.642	588	591	600	rVB	108389	182980	14.65%	2.620%
7	7.962	616	619	628	rBB	481405	789959	63.26%	11.311%
8	8.945	702	705	719	rBV	333889	616359	49.36%	8.825%
9	10.556	843	846	852	rBV	149367	246495	19.74%	3.529%
10	13.208	1074	1078	1081	rBV	804857	1248737	100.00%	17.879%
11	14.671	1203	1206	1212	rBB2	160897	273447	21.90%	3.915%
12	16.408	1356	1358	1368	rVB	319752	460867	36.91%	6.599%
13	17.540	1454	1457	1461	rBV	247436	286800	22.97%	4.106%
14	19.791	1651	1654	1656	rBV	951080	1235340	98.93%	17.688%
15	21.049	1761	1764	1769	rBV	282874	357660	28.64%	5.121%
16	22.672	1904	1906	1913	rBV	224929	275959	22.10%	3.951%
17	23.278	1954	1959	1961	rBV5	5340	16397	1.31%	0.235%


Sum of corrected areas: 6984227

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
Data File : BF077218.D
Acq On : 7 Feb 2015 00:22
Operator : TP/IZ
Sample : G1251-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EXCAVATION-WATER-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

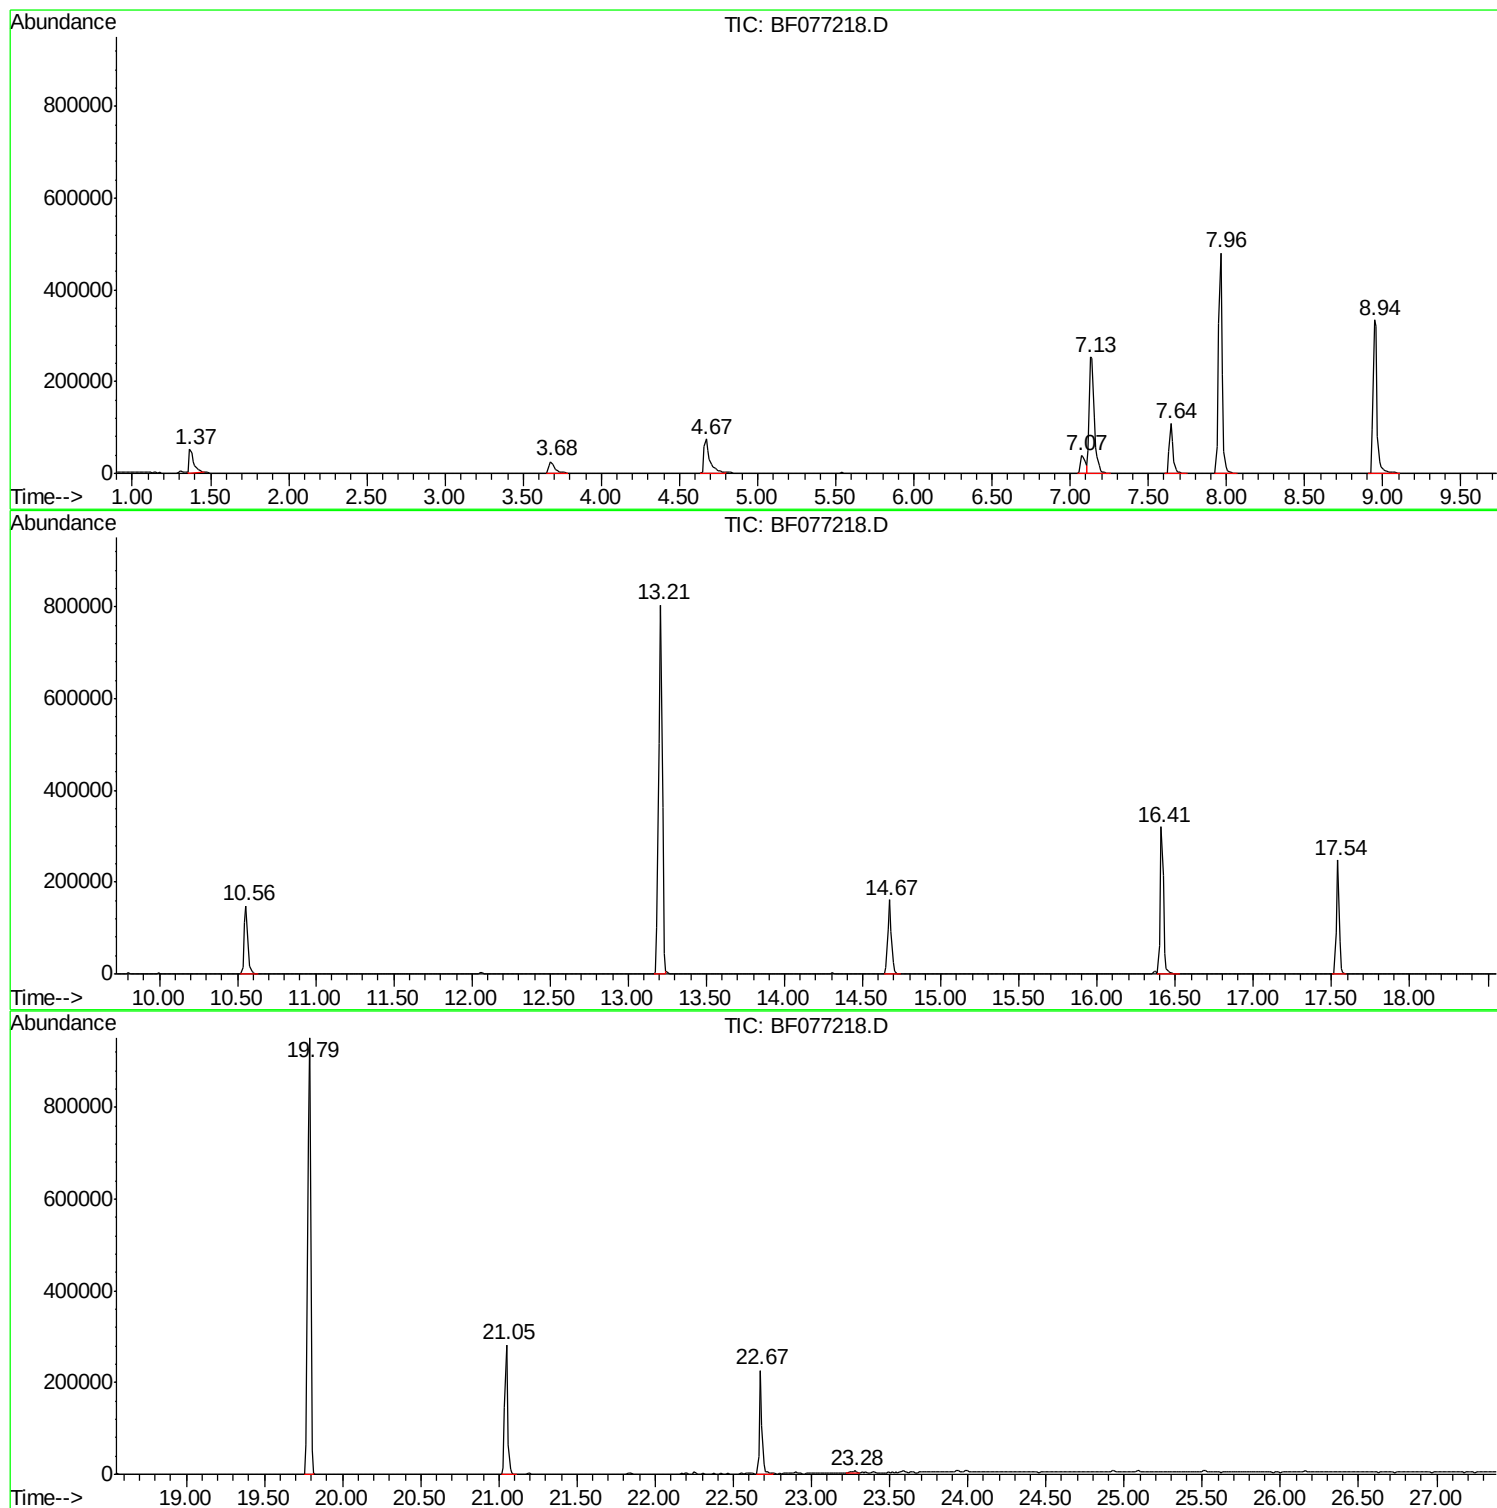

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
Data File : BF077218.D
Acq On : 7 Feb 2015 00:22
Operator : TP/IZ
Sample : G1251-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EXCAVATION-WATER-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020615\
Data File : BF077218.D
Acq On : 7 Feb 2015 00:22
Operator : TP/IZ
Sample : G1251-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EXCAVATION-WATER-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc