

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
 Data File : BF077219.D
 Acq On : 7 Feb 2015 00:56
 Operator : TP/IZ
 Sample : G1245-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SWD-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	40	42	52	rVB	42272	89512	7.53%	1.321%
2	3.676	242	244	256	rBV	18379	53500	4.50%	0.789%
3	4.670	329	331	338	rBV	73373	188896	15.90%	2.787%
4	7.070	539	541	544	rBV	41939	86078	7.25%	1.270%
5	7.139	544	547	557	rVB	257799	533805	44.93%	7.877%
6	7.425	570	572	577	rBV2	5341	12871	1.08%	0.190%
7	7.642	589	591	595	rBV	99631	166681	14.03%	2.460%
8	7.699	595	596	606	rVB2	8858	31310	2.64%	0.462%
9	7.962	615	619	629	rVB	467653	750031	63.13%	11.068%
10	8.956	703	706	715	rBV	322634	579299	48.76%	8.548%
11	10.556	843	846	851	rBV	135905	229538	19.32%	3.387%
12	11.848	954	959	964	rBV2	20132	68380	5.76%	1.009%
13	13.208	1074	1078	1081	rBV	774427	1188045	100.00%	17.531%
14	13.745	1121	1125	1129	rBB2	8210	14937	1.26%	0.220%
15	14.671	1203	1206	1211	rBB2	159313	260948	21.96%	3.851%
16	16.363	1352	1354	1356	rBV	9399	15030	1.27%	0.222%
17	16.408	1356	1358	1366	rVB	321281	463864	39.04%	6.845%
18	17.540	1454	1457	1461	rBV	226840	275435	23.18%	4.064%
19	19.791	1651	1654	1656	rBV	961122	1169941	98.48%	17.264%
20	21.049	1761	1764	1770	rVB	260893	311511	26.22%	4.597%
21	22.683	1905	1907	1914	rBV	196783	273860	23.05%	4.041%
22	23.632	1987	1990	1995	rVB5	4071	13333	1.12%	0.197%


Sum of corrected areas: 6776805

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077219.D
Acq On : 7 Feb 2015 00:56
Operator : TP/IZ
Sample : G1245-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SWD-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

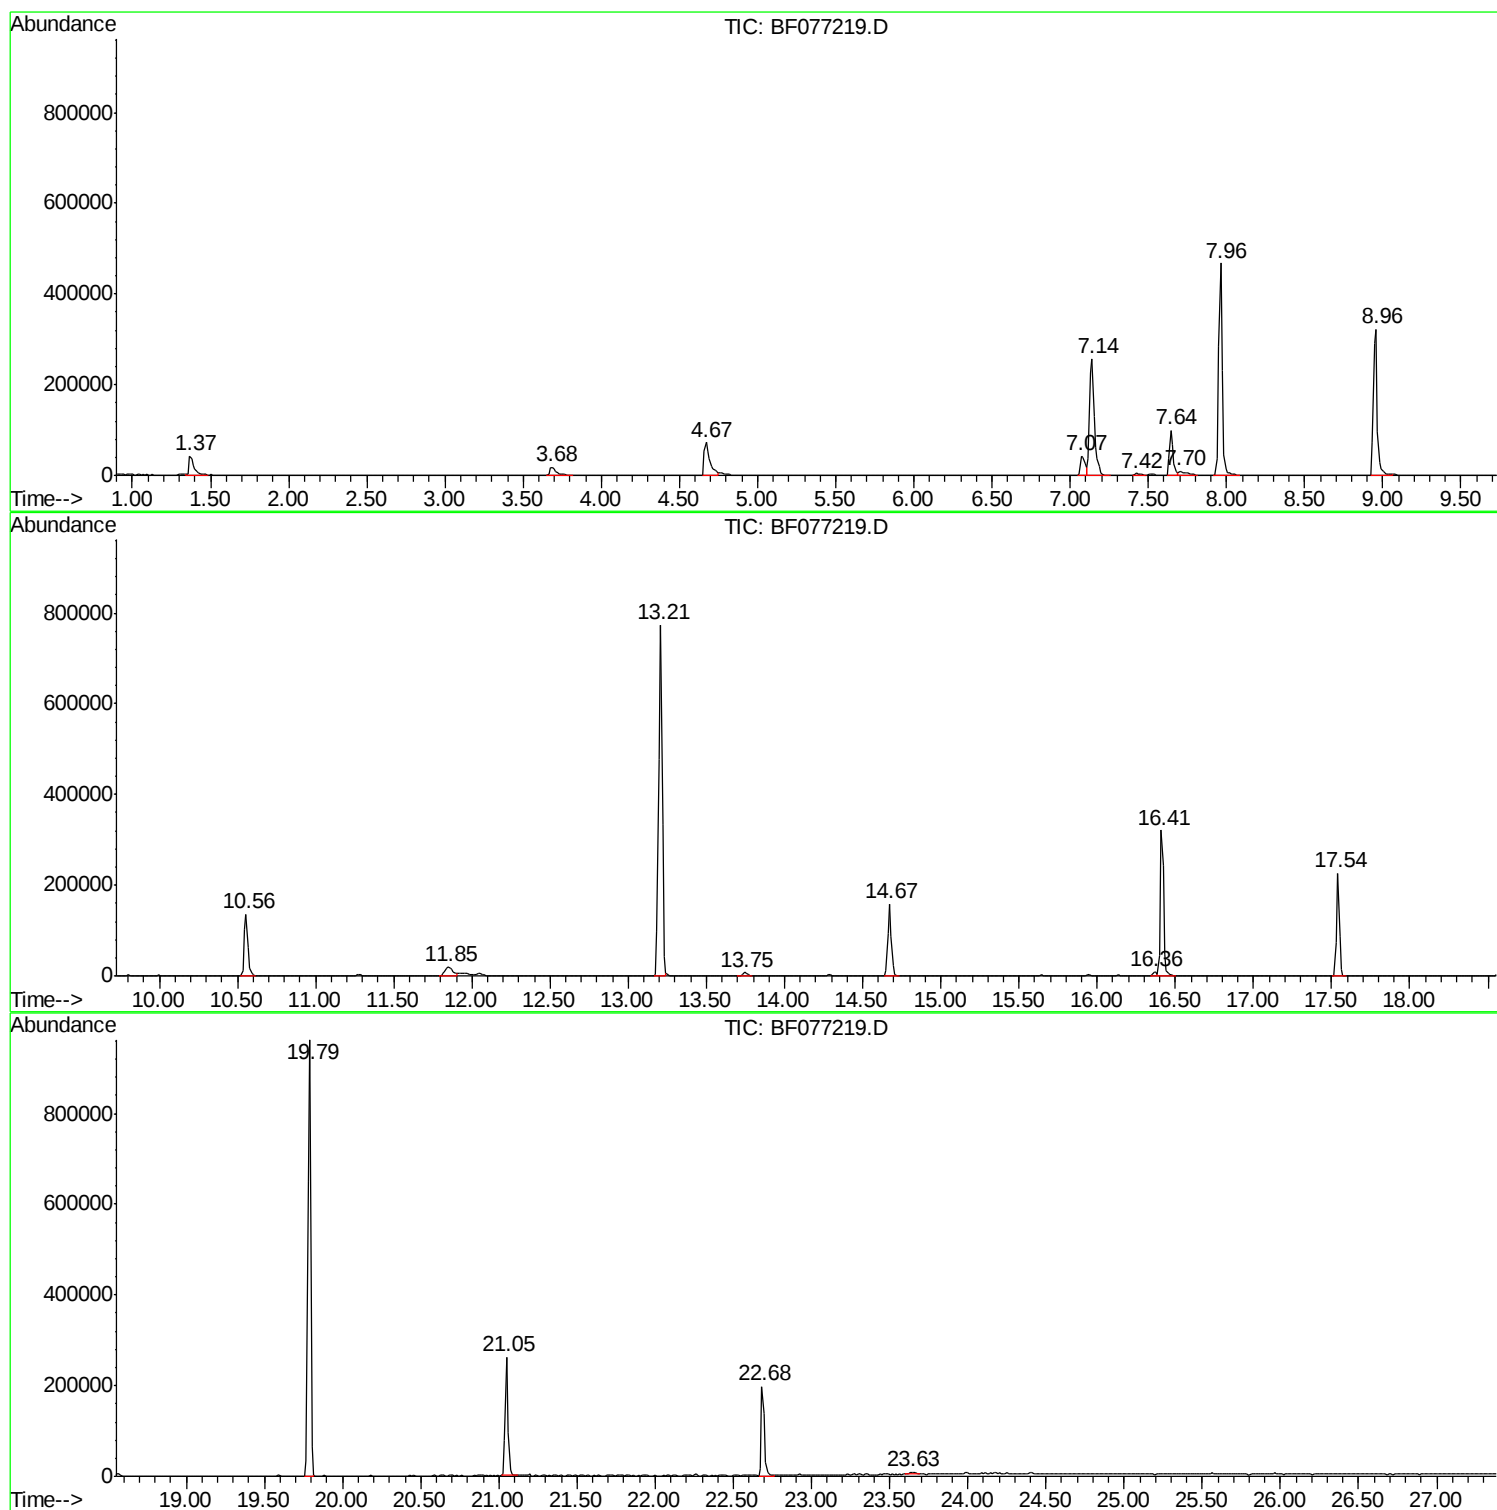

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077219.D
Acq On : 7 Feb 2015 00:56
Operator : TP/IZ
Sample : G1245-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SWD-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.14 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.14	64.05 ng	533805	1,4-Dichlorobenzene-d4	7.64

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Amphetaminil	250	C17H18N2	017590-01-1	10
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

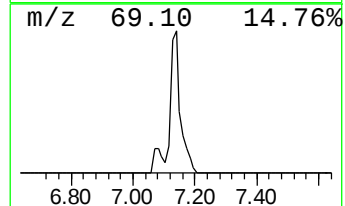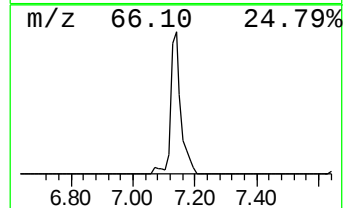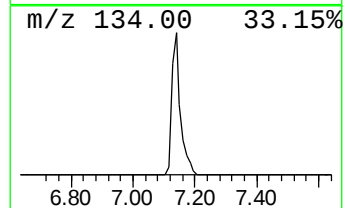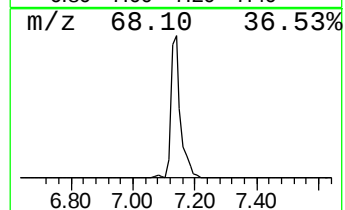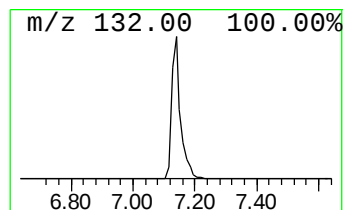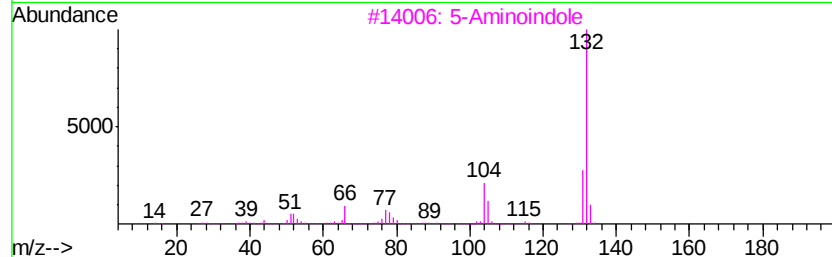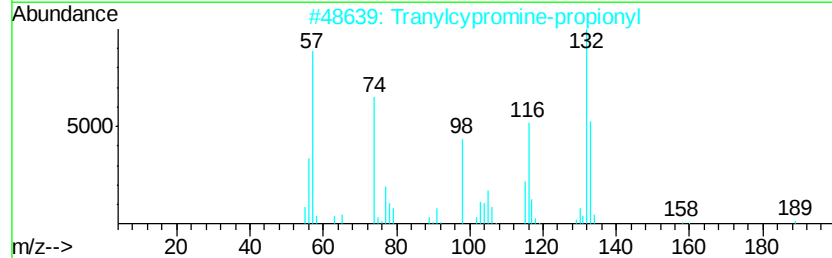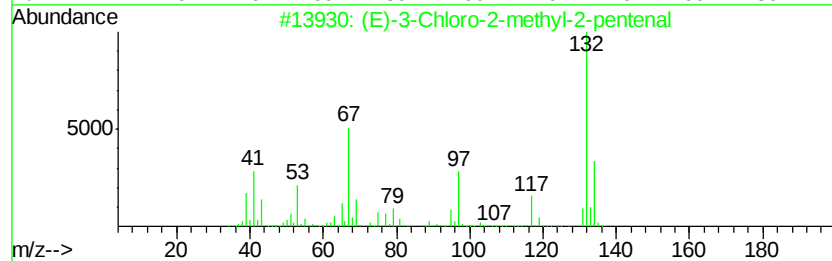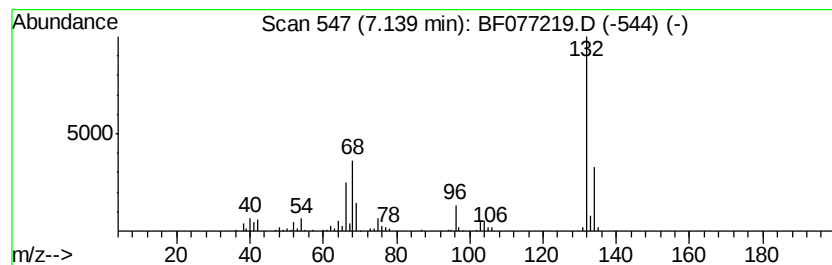

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077219.D
Acq On : 7 Feb 2015 00:56
Operator : TP/IZ
Sample : G1245-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SWD-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 unknown11.85 Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.85	5.96 ng	68380	Naphthalene-d8	10.56

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4,4-(Ethylenedioxy)-2-pentanone	144	C7H12O3	014255-36-8	25
2		Thiophane, propyl-	130	C7H14S	001551-34-4	12
3		Hydrazine, 1-ethyl-1-(1-methylpr...	116	C6H16N2	020325-97-7	9
4		Thiophene, 2-ethyltetrahydro-	116	C6H12S	001551-32-2	9
5		1-Pentanamine	87	C5H13N	000110-58-7	9

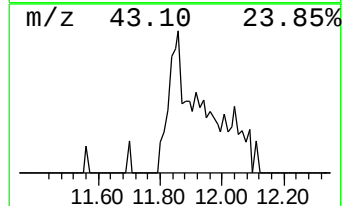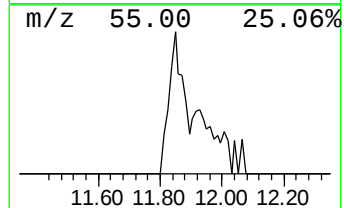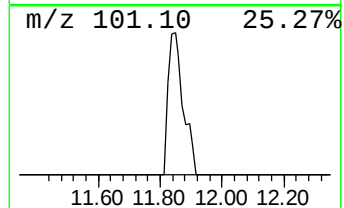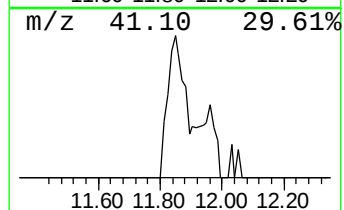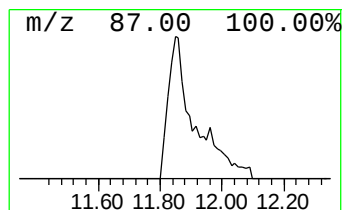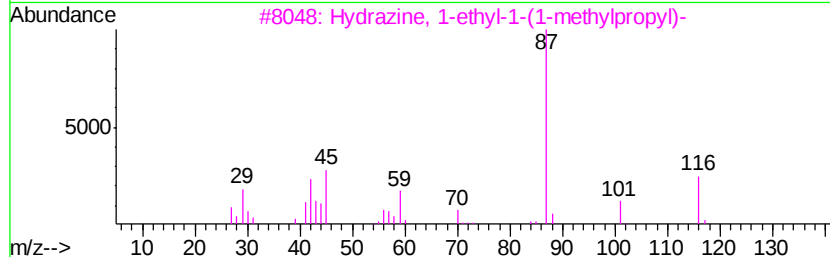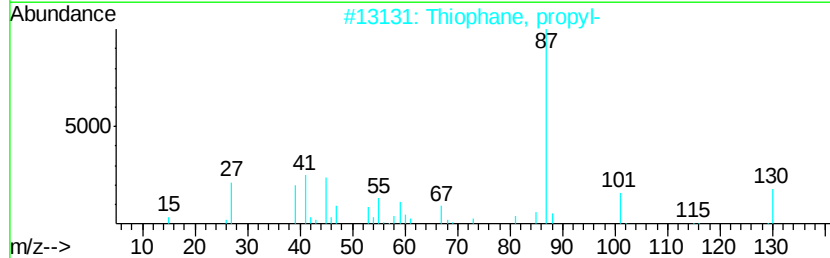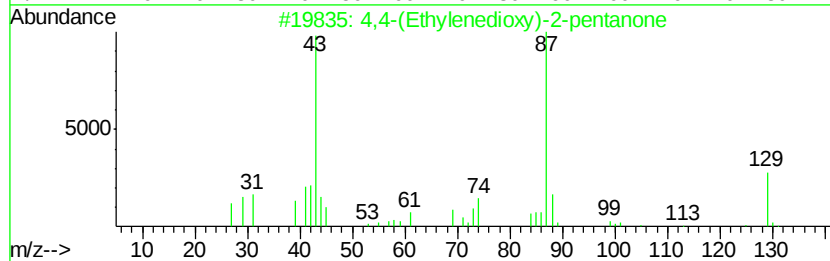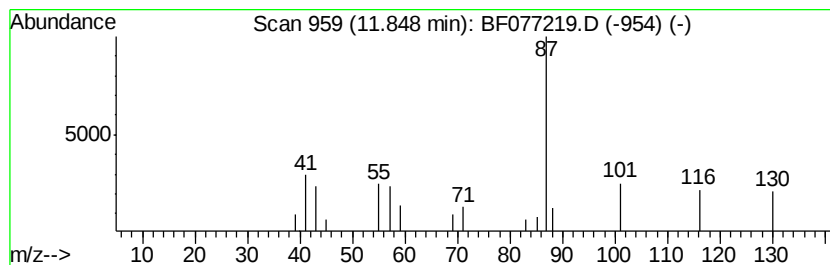

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
Data File : BF077219.D
Acq On : 7 Feb 2015 00:56
Operator : TP/IZ
Sample : G1245-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SWD-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.14	7.14	64.0	ng	533805	1	7.64	166681	20.0
unknown11.85	11.85	6.0	ng	68380	2	10.56	229538	20.0