


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020615\
 Data File : BF077201.D
 Acq On : 6 Feb 2015 12:42
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 30 22:48:24 2015

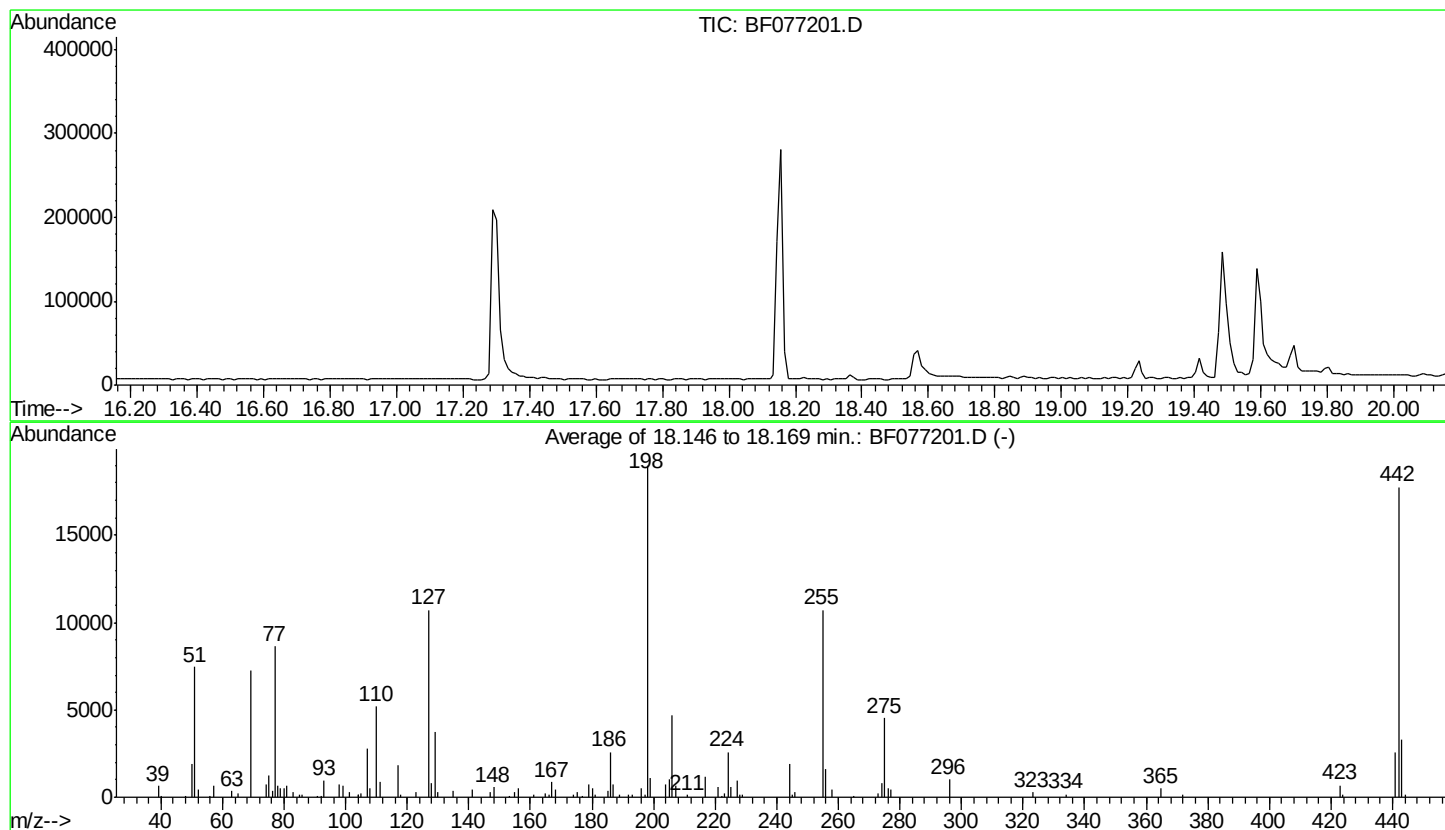

AutoFind: Scans 1510, 1511, 1512; Background Corrected with Scan 1506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	7461	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.2	7257	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.4	10709	PASS
197	198	0.00	2	0.6	123	PASS
198	198	100	100	100.0	18987	PASS
199	198	5	9	5.8	1109	PASS
275	198	10	60	23.8	4510	PASS
365	198	1	100	2.7	507	PASS
441	442	0.01	24	14.5	2574	PASS
442	198	50	100	93.5	17754	PASS
443	442	15	24	18.5	3292	PASS