
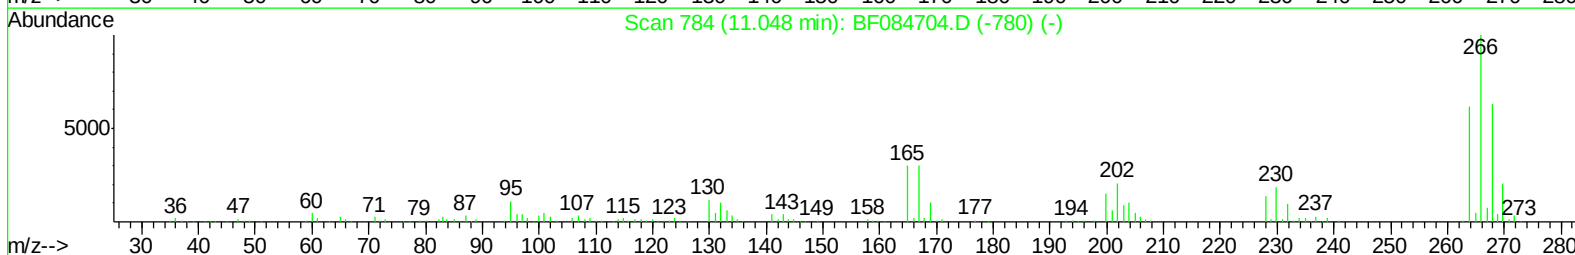
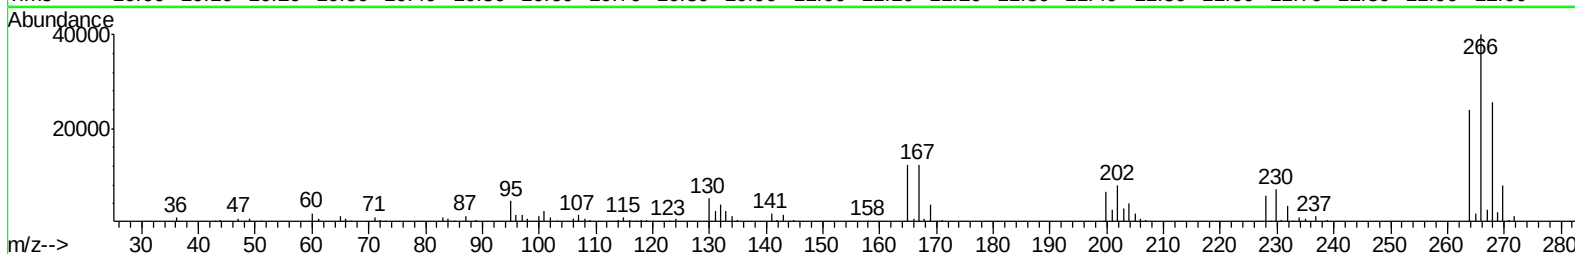


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020616\
Data File : BF084902.D
Acq On : 6 Feb 2016 10:50
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 07:44:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

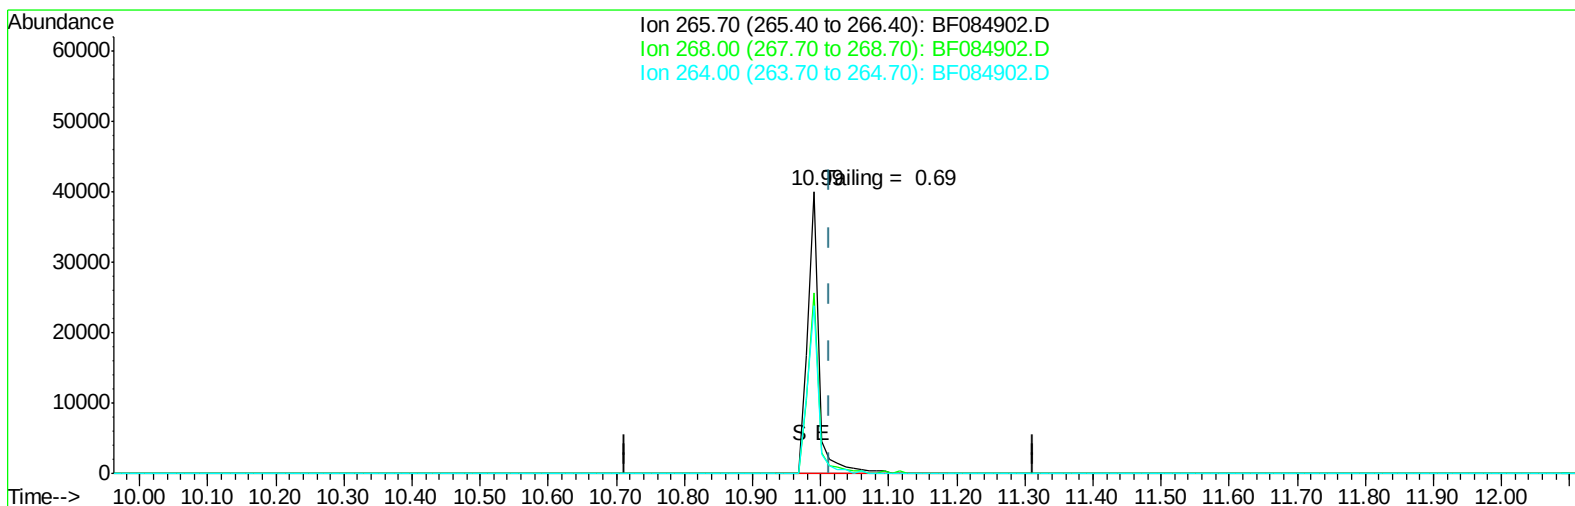

TIC: BF084902.D

(69) Pentachlorophenol (C)




10.991min (-0.023) 38287.19ng

response 46775

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	64.26
264.00	62.70	59.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020616\
Data File : BF084902.D
Acq On : 6 Feb 2016 10:50
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 07:44:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

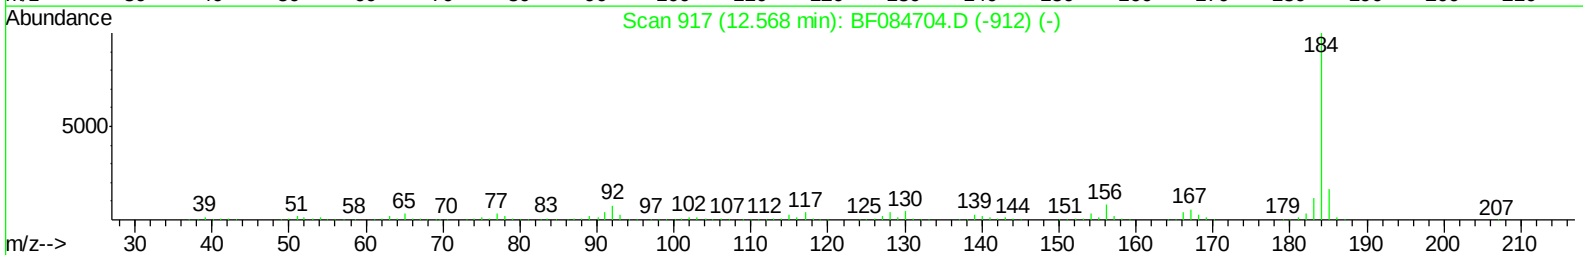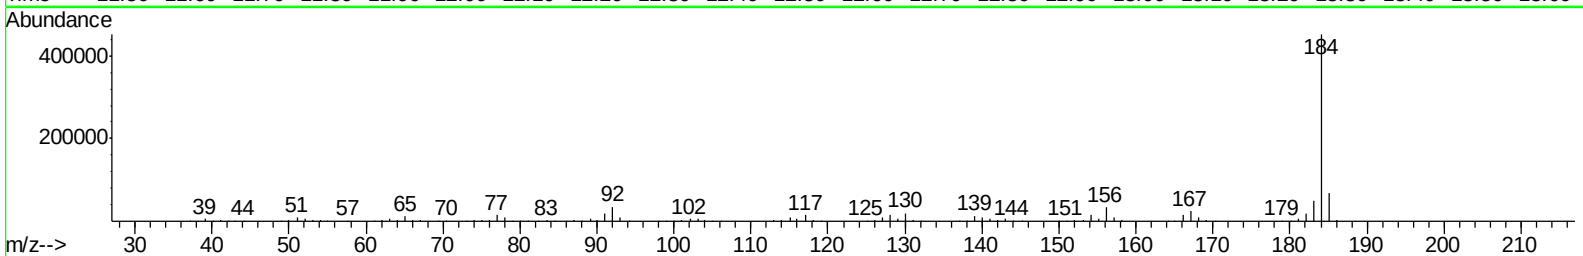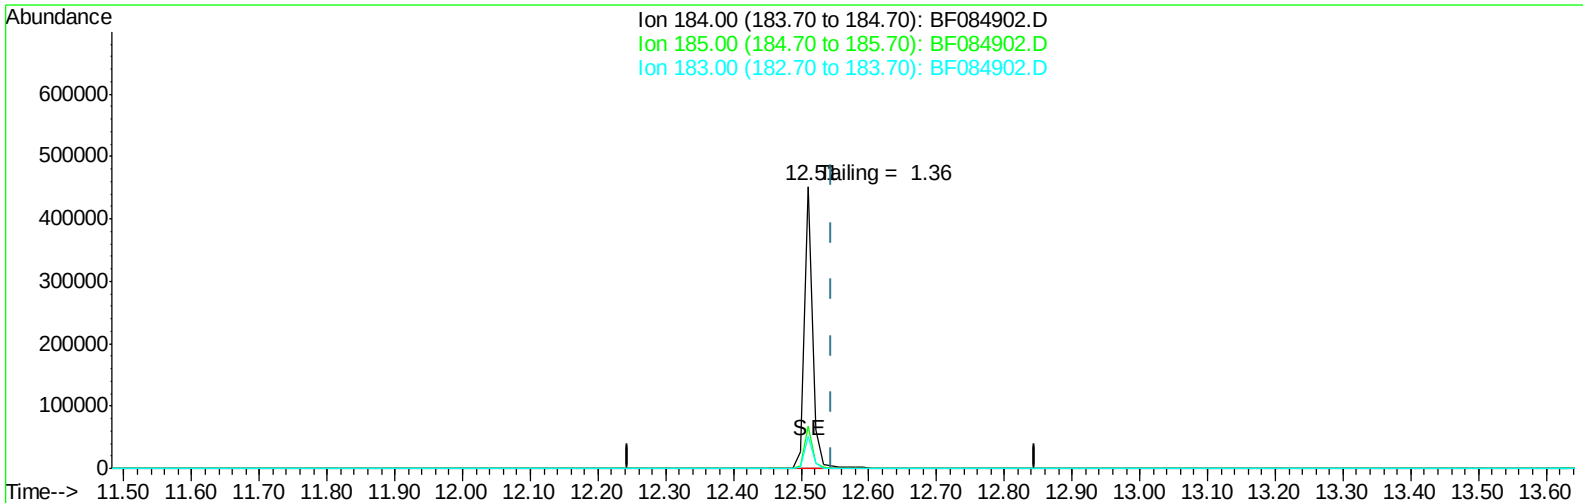

TIC: BF084902.D

(76) Benzidine

12.511min (-0.034) 0.00ng

response 383738

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.23
183.00	12.30	11.37
0.00	0.00	0.00