


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020616\
 Data File : BF084902.D
 Acq On : 6 Feb 2016 10:50
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 14:16:01 2016

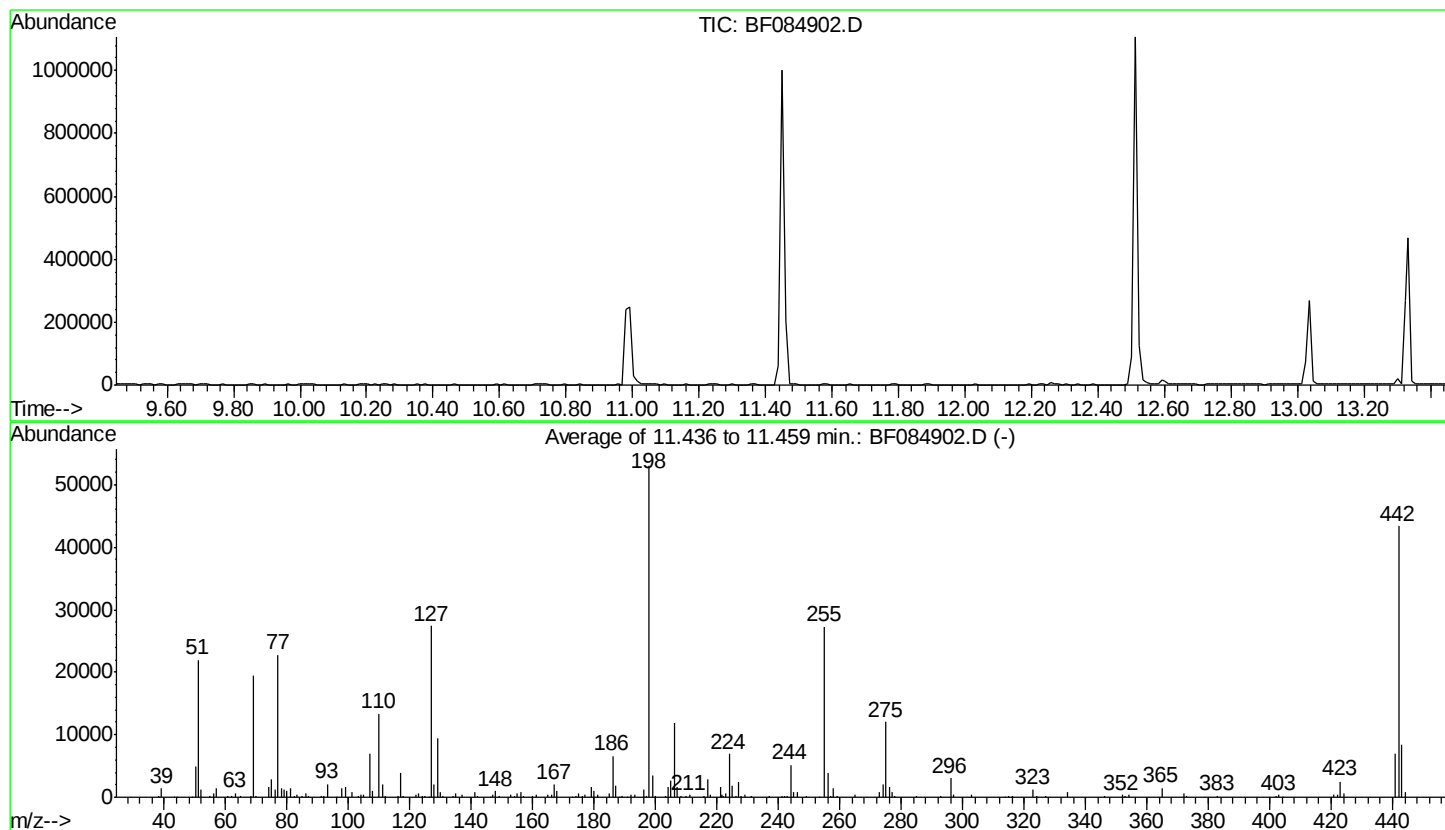

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	21995	PASS
68	69	0.00	2	1.6	304	PASS
69	198	0.00	100	36.6	19412	PASS
70	69	0.00	2	0.6	113	PASS
127	198	10	80	51.6	27357	PASS
197	198	0.00	2	0.5	244	PASS
198	198	100	100	100.0	53053	PASS
199	198	5	9	6.5	3464	PASS
275	198	10	60	22.7	12054	PASS
365	198	1	100	2.8	1465	PASS
441	442	0.01	24	16.3	7073	PASS
442	198	50	100	81.8	43396	PASS
443	442	15	24	19.4	8407	PASS