
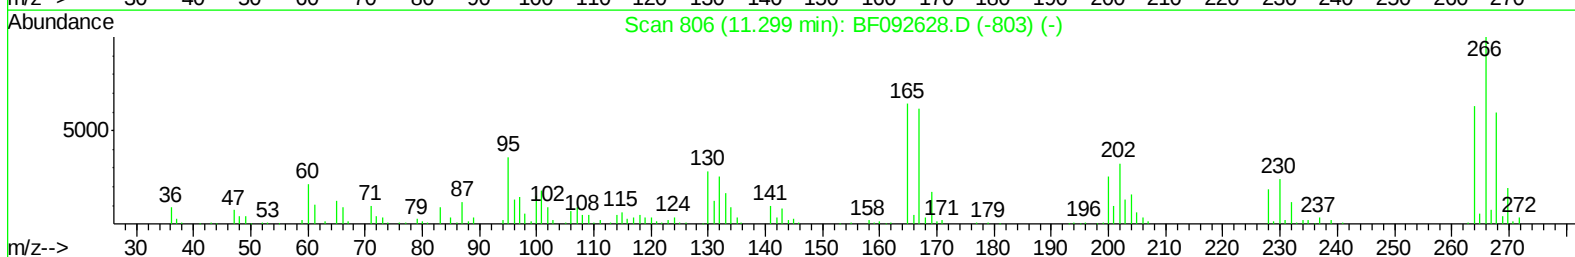
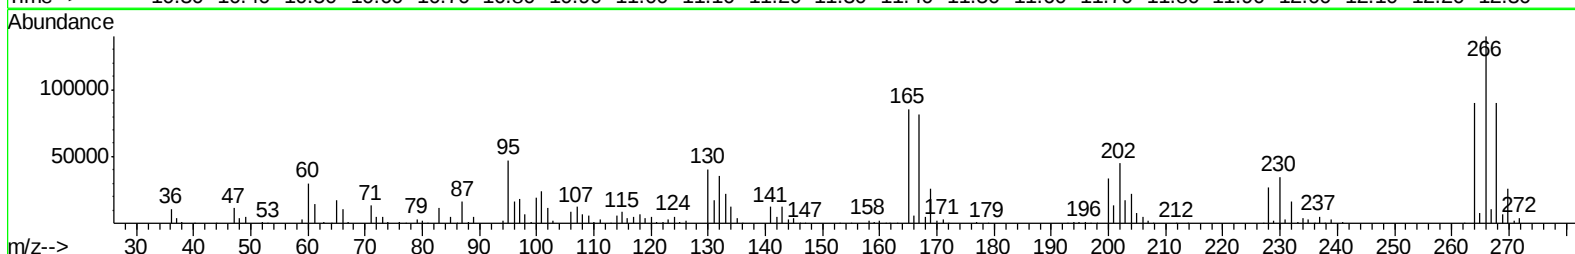


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020617\
Data File : BF092797.D
Acq On : 6 Feb 2017 15:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:02:58 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 01:19:37 2017
Response via : Initial Calibration

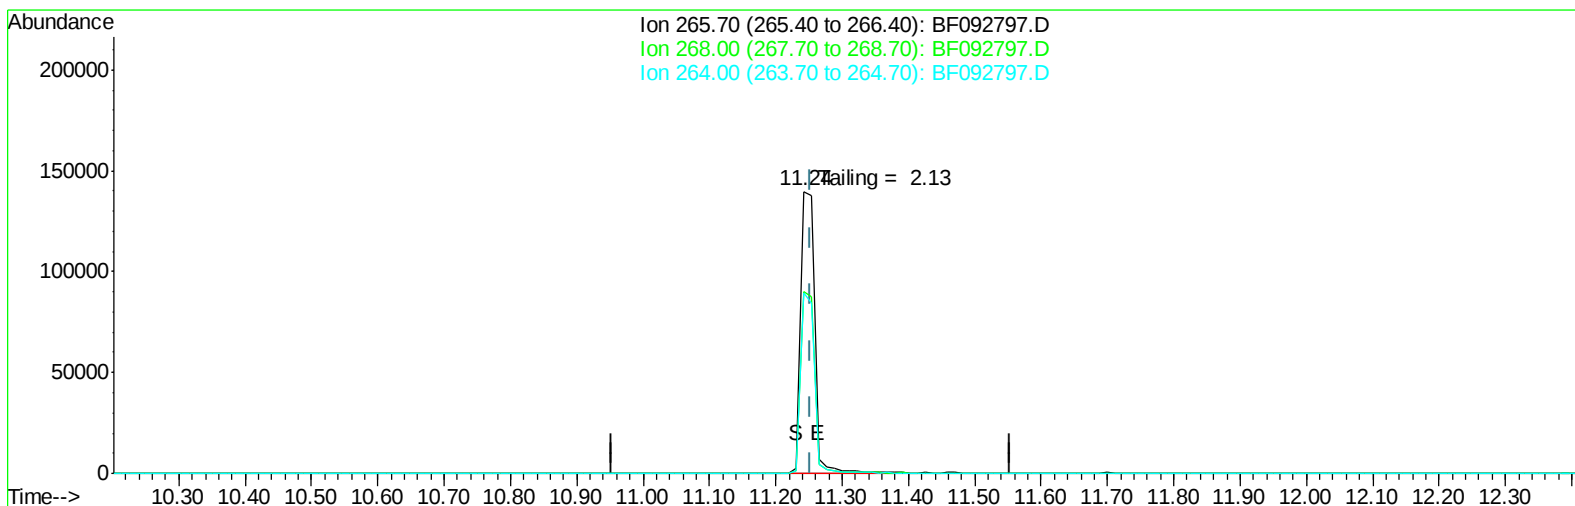

TIC: BF092797.D

(69) Pentachlorophenol (C)




11.242min (-0.011) 0.00ng

response 205301

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.68
264.00	62.90	64.28
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020617\
Data File : BF092797.D
Acq On : 6 Feb 2017 15:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:02:58 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 01:19:37 2017
Response via : Initial Calibration

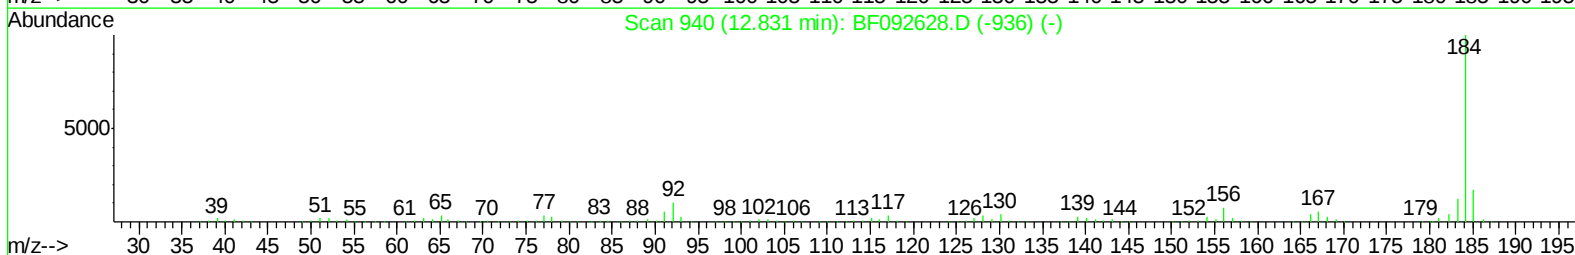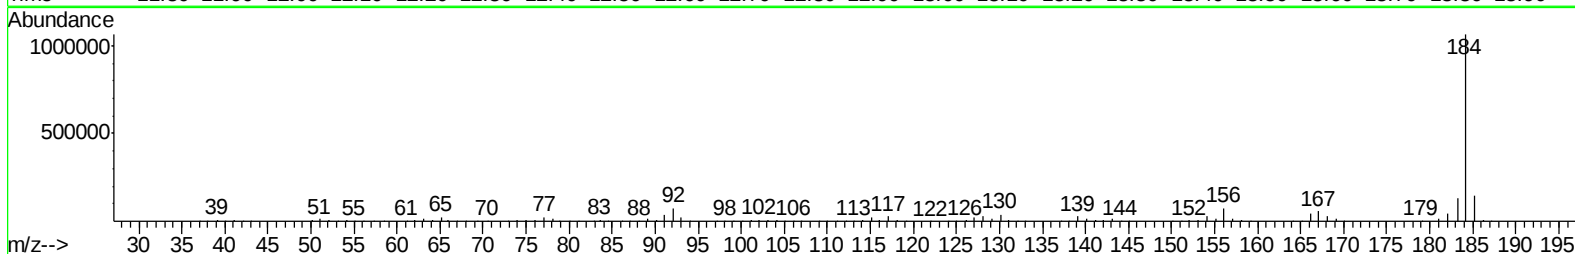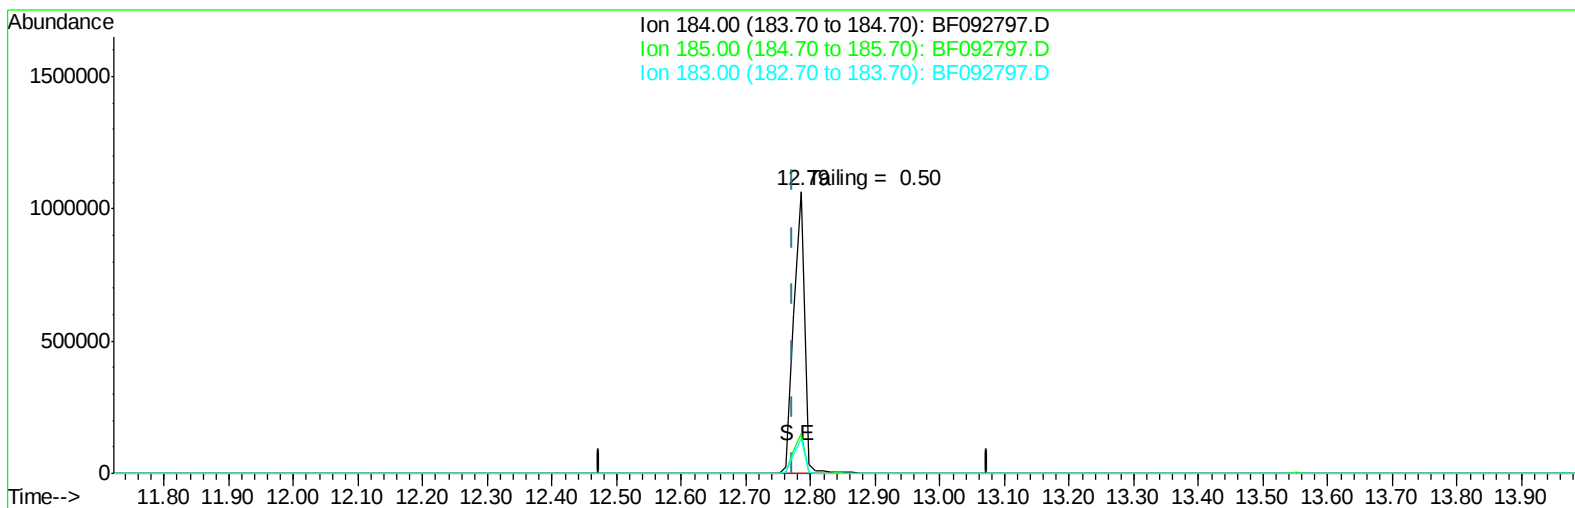

TIC: BF092797.D

(76) Benzidine

12.785min (+0.012) 22214.67ng

response 1214523

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.08
183.00	11.50	12.32
0.00	0.00	0.00