


Data Path : Z:\HPCHEM1\BNA F\Data\BF020617\
 Data File : BF092797.D
 Acq On : 6 Feb 2017 15:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

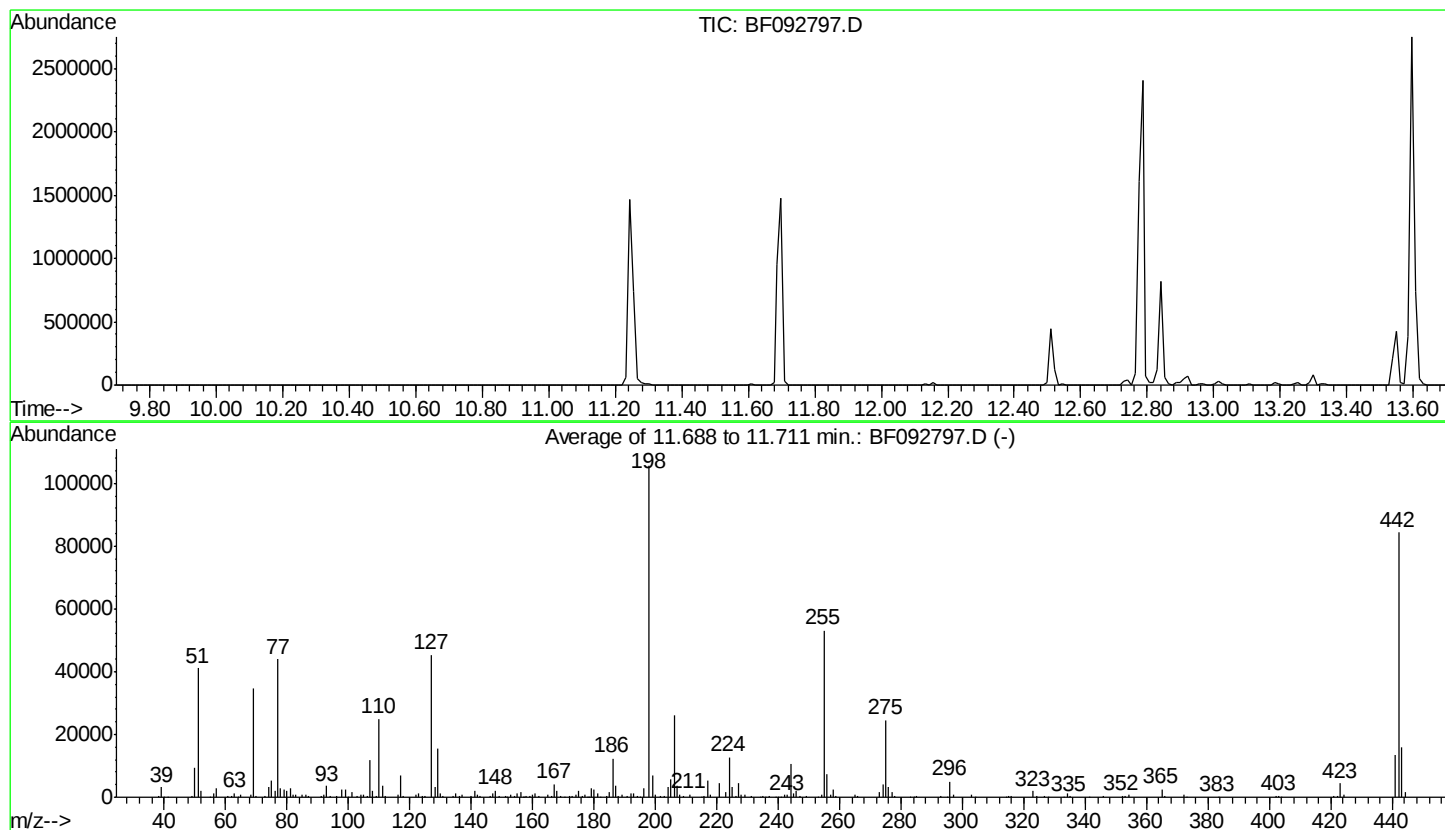

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	41021	PASS
68	69	0.00	2	1.9	642	PASS
69	198	0.00	100	32.9	34697	PASS
70	69	0.00	2	0.8	285	PASS
127	198	10	80	42.9	45331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105611	PASS
199	198	5	9	6.6	7008	PASS
275	198	10	60	23.2	24518	PASS
365	198	1	100	2.3	2454	PASS
441	442	0.01	24	16.1	13545	PASS
442	198	50	100	79.7	84208	PASS
443	442	15	24	18.9	15934	PASS