
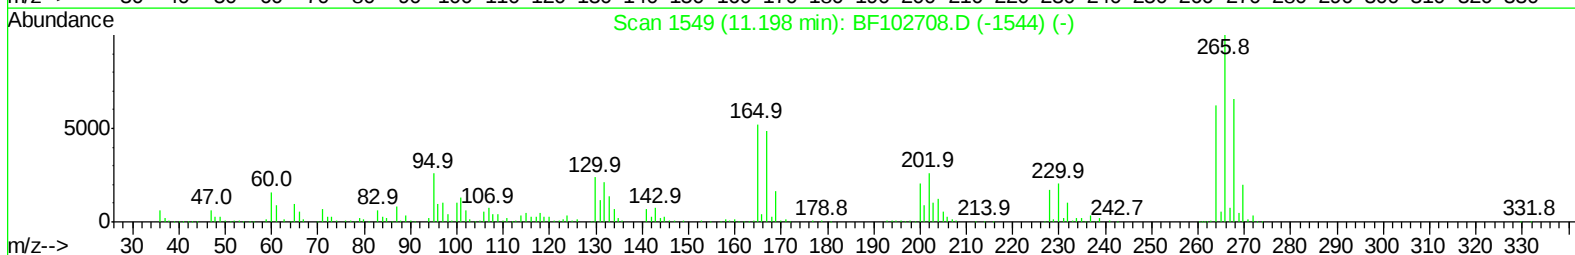
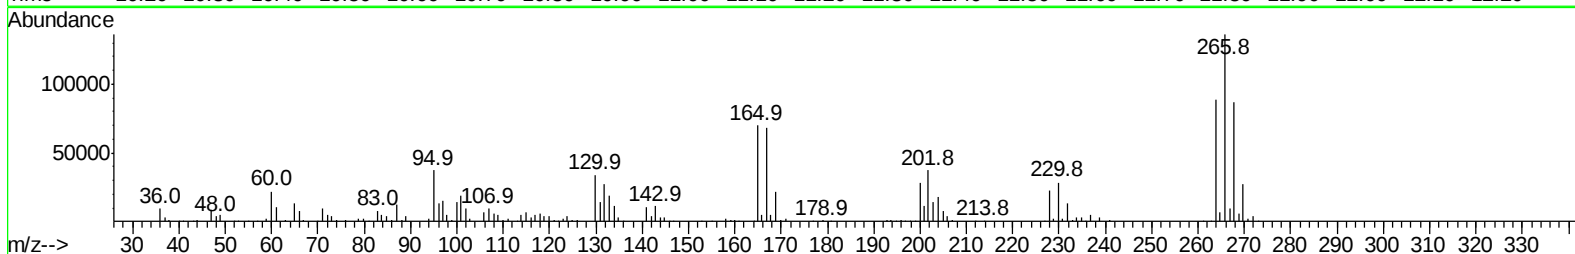


Data Path : U:\HPCHEM1\BNA F\DATA\BF020618\
 Data File : BF102771.D
 Acq On : 6 Feb 2018 9:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 02:53:43 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 12:44:16 2018
 Response via : Initial Calibration

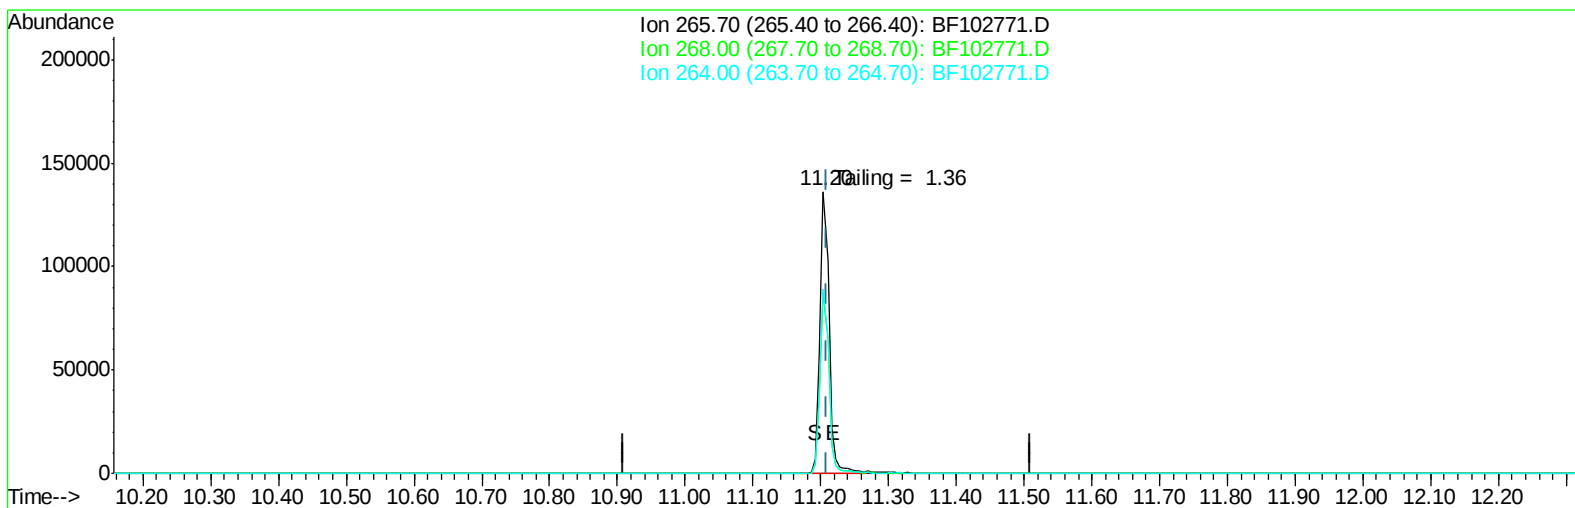

TIC: BF102771.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 81843.58ng

response 123344

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.94
264.00	61.90	65.33
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF020618\
Data File : BF102771.D
Acq On : 6 Feb 2018 9:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 02:53:43 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

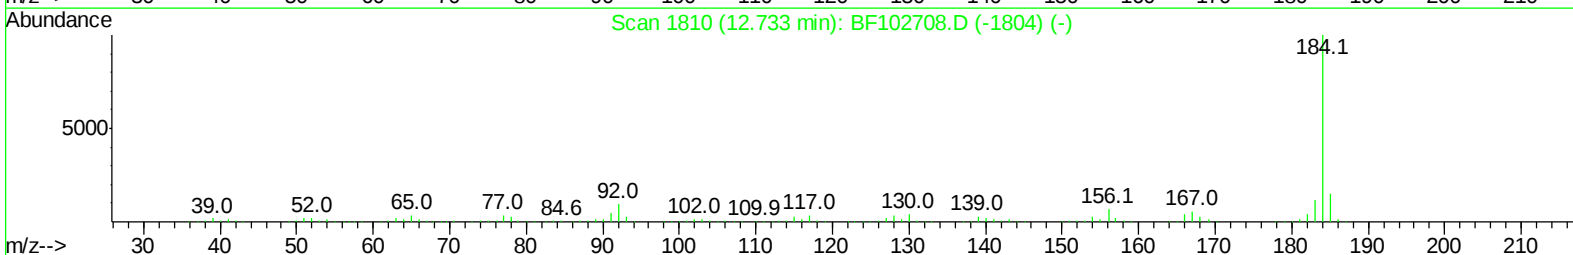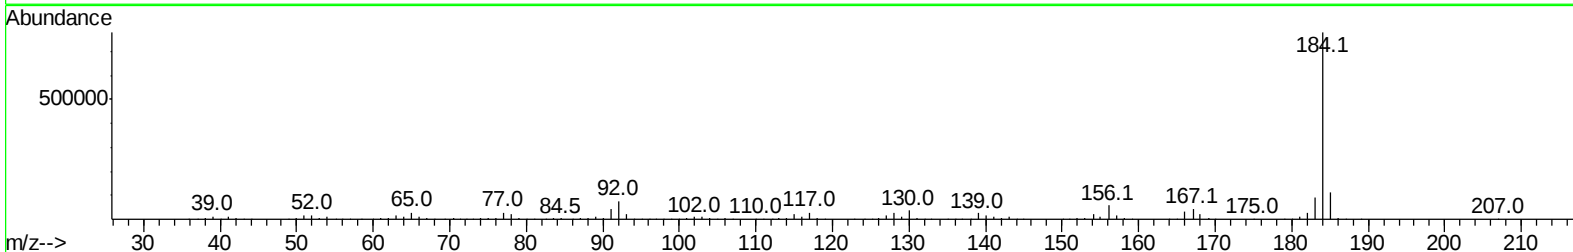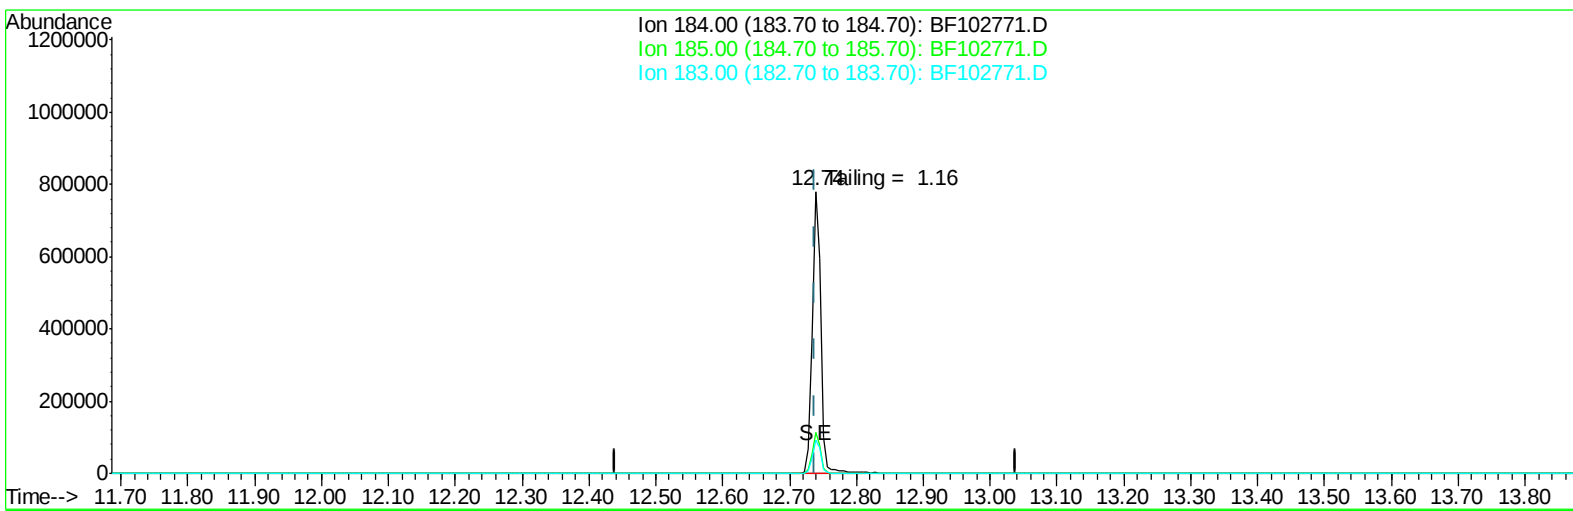

TIC: BF102771.D

(76) Benzidine

12.739min (+0.000) 58819.37ng

response 708278

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.41
183.00	11.60	11.86
0.00	0.00	0.00