
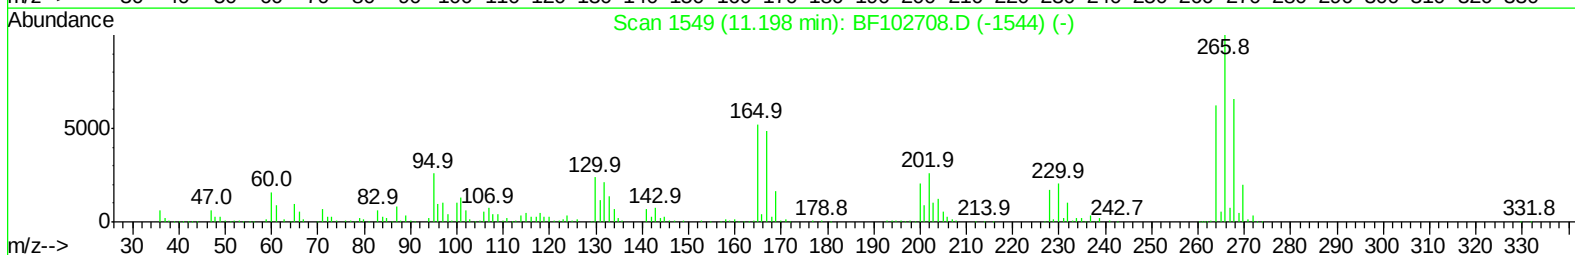
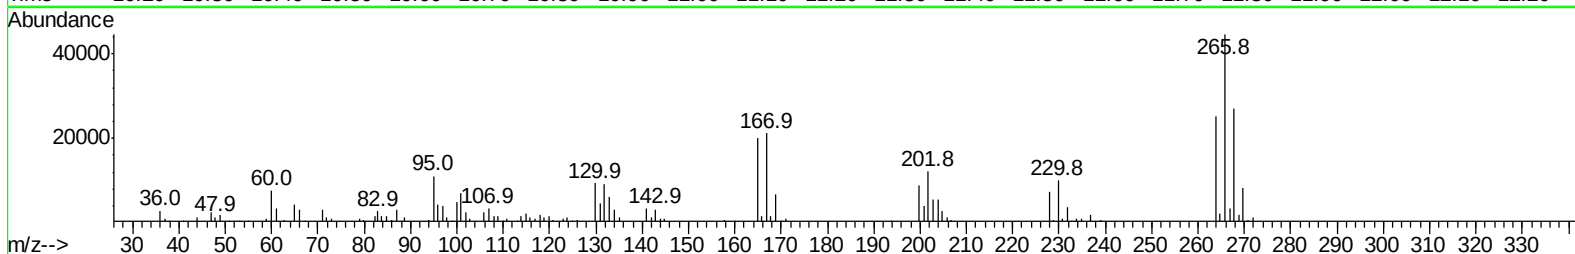


Data Path : U:\HPCHEM1\BNA F\DATA\BF020618\
Data File : BF102798.D
Acq On : 6 Feb 2018 22:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 02:55:04 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

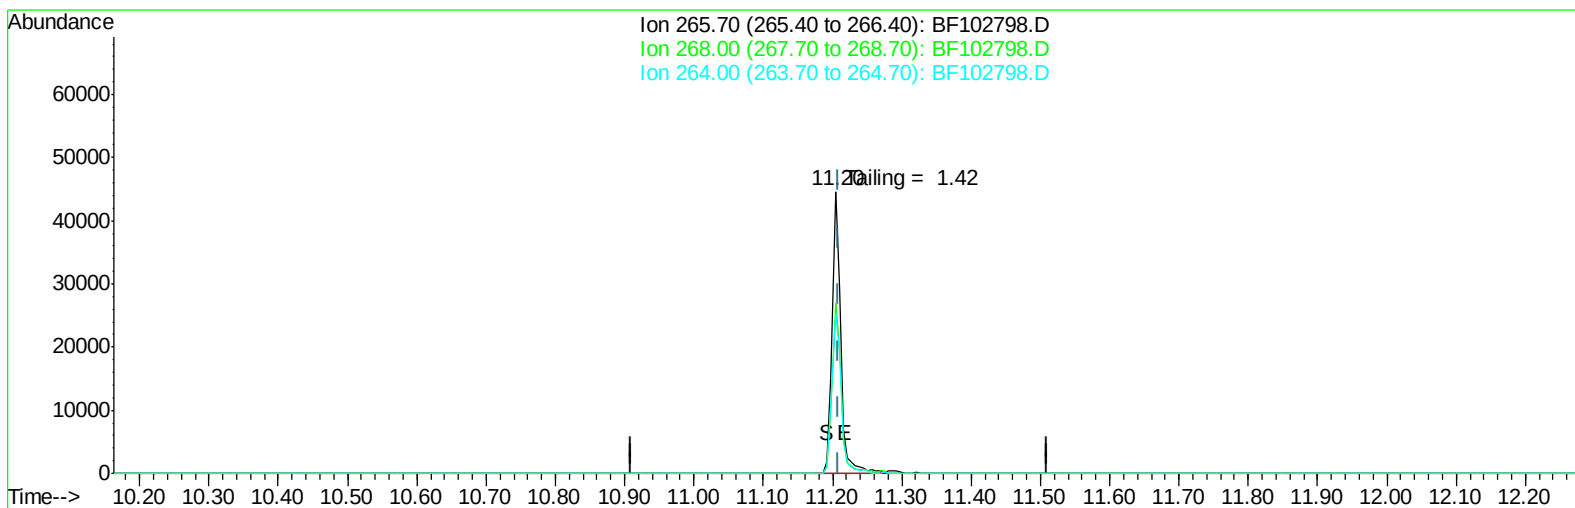

TIC: BF102798.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 12127.46ng

response 37800

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.33
264.00	61.90	56.80
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF020618\
Data File : BF102798.D
Acq On : 6 Feb 2018 22:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 02:55:04 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

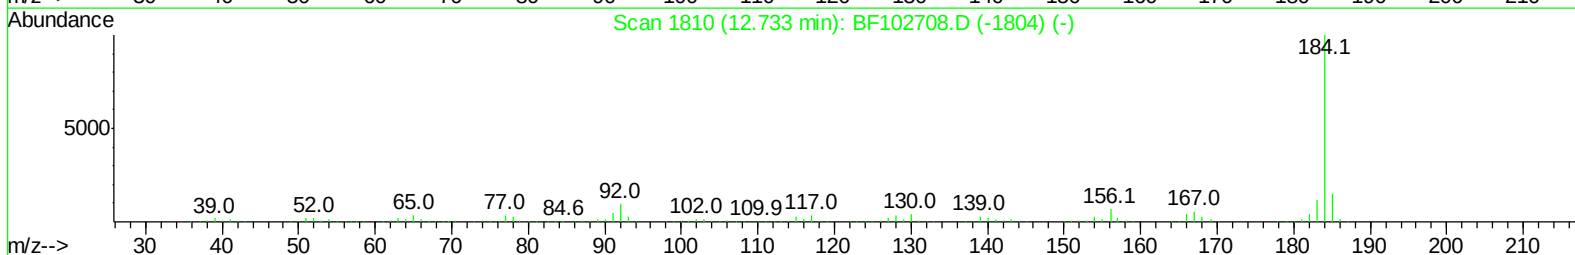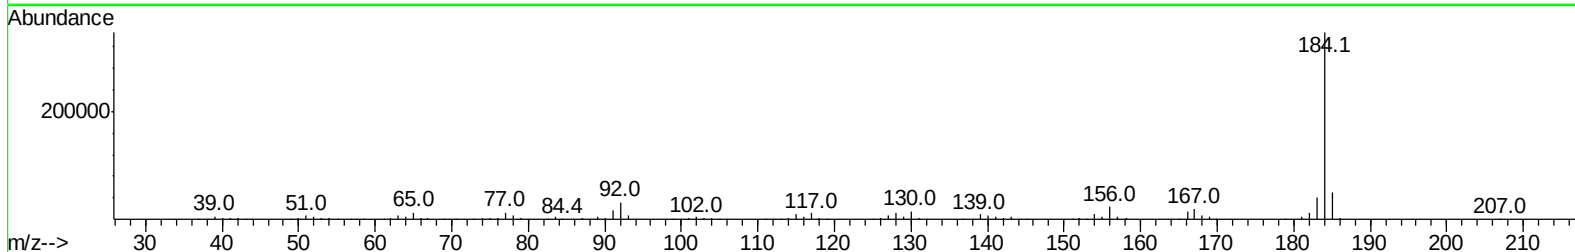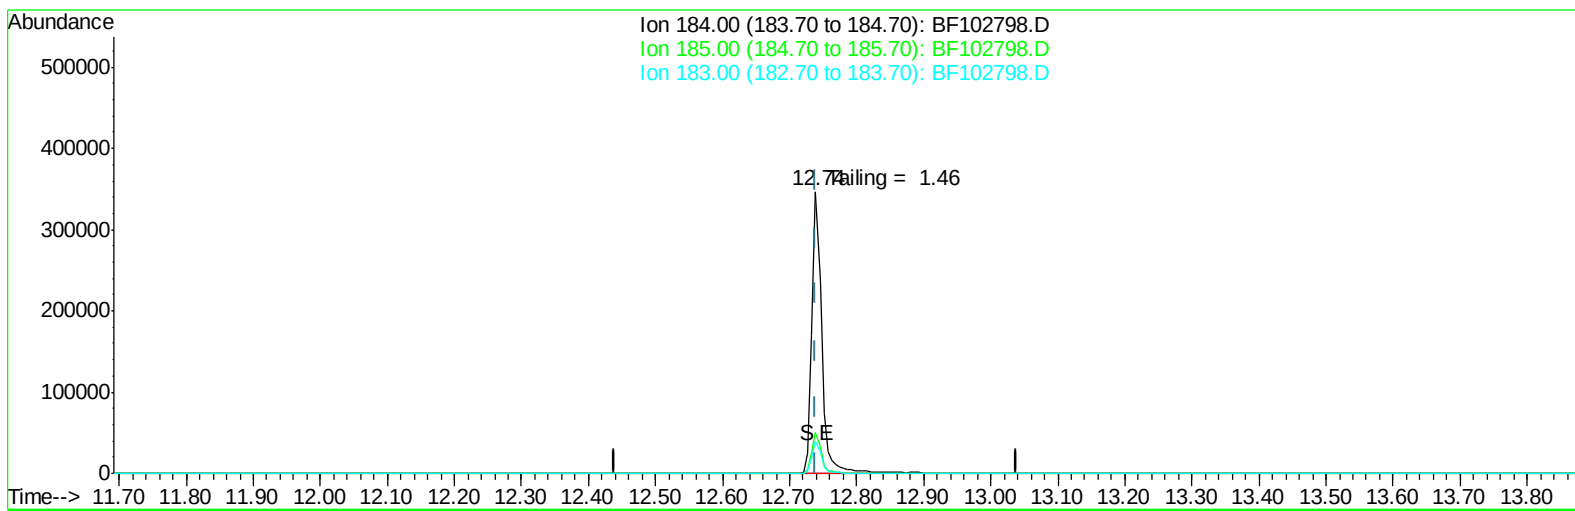

TIC: BF102798.D

(76) Benzidine

12.739min (-0.000) 6909.46ng

response 337884

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.62
183.00	11.60	11.50
0.00	0.00	0.00