

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020618\
 Data File : BF102778.D
 Acq On : 6 Feb 2018 12:36
 Operator : SJ/JU
 Sample : J1454-10DL 4X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 8-SAN-8-EW(4-7)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	4	8	28	rVB	142226	271098	8.38%	0.550%
2	5.092	508	511	515	rVB	44496	46041	1.42%	0.093%
3	5.486	574	578	586	rVB	1286785	1090178	33.69%	2.212%
4	6.128	682	687	690	rBV2	40203	52626	1.63%	0.107%
5	6.492	745	749	754	rBV	1179452	1159888	35.85%	2.354%
6	6.645	771	775	778	rVB	1320794	1105383	34.16%	2.243%
7	6.710	783	786	789	rBV4	44982	55456	1.71%	0.113%
8	6.880	811	815	819	rVB	1543236	1299829	40.17%	2.638%
9	7.033	836	841	844	rBV	995722	860546	26.60%	1.746%
10	7.198	864	869	871	rBV2	33915	41541	1.28%	0.084%
11	7.275	876	882	885	rBV3	64742	71867	2.22%	0.146%
12	7.410	900	905	906	rBV3	51249	58397	1.80%	0.118%
13	7.439	906	910	913	rVV	748273	695996	21.51%	1.412%
14	7.469	913	915	919	rVV	75142	72588	2.24%	0.147%
15	7.522	919	924	927	rVB5	31445	52175	1.61%	0.106%
16	7.586	927	935	937	rBV5	20342	42731	1.32%	0.087%
17	7.904	986	989	992	rBV3	40760	48765	1.51%	0.099%
18	8.163	1026	1033	1035	rBV	1967745	1827396	56.48%	3.708%
19	8.186	1035	1037	1040	rVB	1269965	932981	28.83%	1.893%
20	8.216	1040	1042	1044	rBV	72883	58915	1.82%	0.120%
21	8.451	1074	1082	1086	rBV7	64893	108618	3.36%	0.220%
22	8.516	1088	1093	1095	rBV2	53235	63093	1.95%	0.128%
23	8.580	1101	1104	1106	rBV	96652	80779	2.50%	0.164%
24	8.751	1130	1133	1136	rBV	145198	128008	3.96%	0.260%
25	8.874	1151	1154	1158	rVB	443058	331898	10.26%	0.673%
26	8.974	1167	1171	1175	rVB	288534	243092	7.51%	0.493%
27	9.033	1178	1181	1184	rBV4	43899	66240	2.05%	0.134%
28	9.110	1191	1194	1198	rBV5	40019	50423	1.56%	0.102%
29	9.180	1203	1206	1209	rVV	118516	108116	3.34%	0.219%
30	9.233	1212	1215	1220	rBV	1310262	1107463	34.23%	2.247%
31	9.316	1225	1229	1231	rBV	221161	229904	7.11%	0.467%
32	9.339	1231	1233	1237	rVB	103659	95709	2.96%	0.194%
33	9.433	1246	1249	1254	rBV	97570	93779	2.90%	0.190%
34	9.504	1257	1261	1264	rVV2	136463	178105	5.50%	0.361%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020618\
 Data File : BF102778.D
 Acq On : 6 Feb 2018 12:36
 Operator : SJ/JU
 Sample : J1454-10DL 4X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 8-SAN-8-EW(4-7)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.574	1270	1273	1275	rBV	217877	176107	5.44%	0.357%
36	9.604	1275	1278	1280	rVB	120653	107135	3.31%	0.217%
37	9.627	1280	1282	1286	rBV3	220478	238648	7.38%	0.484%
38	9.692	1290	1293	1295	rBV	131257	110955	3.43%	0.225%
39	9.780	1305	1308	1312	rBV4	92324	109292	3.38%	0.222%
40	9.845	1312	1319	1323	rBV	270902	334650	10.34%	0.679%
41	9.921	1326	1332	1335	rVV	1818840	1741698	53.83%	3.534%
42	9.951	1335	1337	1340	rVV	1071032	807098	24.94%	1.638%
43	9.980	1340	1342	1346	rVB2	76918	83180	2.57%	0.169%
44	10.021	1346	1349	1353	rBV	103218	128012	3.96%	0.260%
45	10.074	1353	1358	1360	rBV4	122324	166649	5.15%	0.338%
46	10.121	1363	1366	1370	rVV2	597375	565914	17.49%	1.148%
47	10.163	1370	1373	1377	rVB4	143785	180415	5.58%	0.366%
48	10.233	1382	1385	1388	rBV	183215	184728	5.71%	0.375%
49	10.263	1388	1390	1392	rBV2	105202	80458	2.49%	0.163%
50	10.327	1397	1401	1402	rBV2	168338	191348	5.91%	0.388%
51	10.345	1402	1404	1406	rVB	340796	241406	7.46%	0.490%
52	10.374	1406	1409	1411	rBV3	58464	67313	2.08%	0.137%
53	10.468	1421	1425	1428	rBV	827858	809834	25.03%	1.643%
54	10.515	1431	1433	1434	rVV	85038	68214	2.11%	0.138%
55	10.557	1437	1440	1446	rVV3	260170	474778	14.67%	0.963%
56	10.621	1449	1451	1454	rVB	212923	187741	5.80%	0.381%
57	10.686	1459	1462	1463	rBV3	91026	96050	2.97%	0.195%
58	10.704	1463	1465	1469	rVB	673221	556218	17.19%	1.129%
59	10.833	1481	1487	1489	rBV3	515277	768667	23.76%	1.560%
60	11.010	1515	1517	1520	rVV2	136089	104681	3.24%	0.212%
61	11.045	1520	1523	1526	rVB4	148145	149533	4.62%	0.303%
62	11.210	1549	1551	1554	rVB3	143019	120860	3.74%	0.245%
63	11.268	1558	1561	1563	rVV	393336	388851	12.02%	0.789%
64	11.298	1563	1566	1572	rVB2	770116	846826	26.17%	1.718%
65	11.410	1581	1585	1587	rBV	1373941	1506300	46.55%	3.057%
66	11.433	1587	1589	1592	rVV	3448873	3162889	97.75%	6.418%
67	11.486	1595	1598	1600	rVB	1121573	984582	30.43%	1.998%
68	11.515	1600	1603	1605	rBV	262406	245618	7.59%	0.498%
69	11.639	1621	1624	1628	rVB2	500067	623817	19.28%	1.266%
70	11.698	1631	1634	1636	rVB2	407669	386357	11.94%	0.784%
71	11.910	1667	1670	1672	rBV	443687	422788	13.07%	0.858%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020618\
 Data File : BF102778.D
 Acq On : 6 Feb 2018 12:36
 Operator : SJ/JU
 Sample : J1454-10DL 4X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 8-SAN-8-EW(4-7)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.933	1672	1674	1679	rVB	610840	685705	21.19%	1.391%
73	12.021	1686	1689	1691	rBV2	601042	602194	18.61%	1.222%
74	12.104	1701	1703	1706	rBV2	395846	308942	9.55%	0.627%
75	12.204	1718	1720	1722	rBV	279339	230857	7.13%	0.468%
76	12.457	1761	1763	1766	rBV2	328783	326714	10.10%	0.663%
77	12.492	1767	1769	1775	rVB3	418702	444944	13.75%	0.903%
78	12.627	1788	1792	1795	rVB	2744121	2531121	78.23%	5.136%
79	12.857	1825	1831	1836	rBV	2432872	3235600	100.00%	6.566%
80	12.992	1852	1854	1863	rVB2	738559	876700	27.10%	1.779%
81	13.180	1884	1886	1889	rVB	665185	503659	15.57%	1.022%
82	13.245	1895	1897	1900	rBV	386491	342099	10.57%	0.694%
83	14.045	2029	2033	2037	rBV3	1567858	2302405	71.16%	4.672%
84	14.080	2037	2039	2046	rVB	1303233	1140496	35.25%	2.314%
85	15.103	2209	2213	2216	rBV	1019275	1613849	49.88%	3.275%
86	15.409	2263	2265	2271	rVB	649391	786175	24.30%	1.595%
87	15.474	2272	2276	2282	rVB	954791	1345790	41.59%	2.731%
88	15.539	2283	2287	2290	rBV	711048	977103	30.20%	1.983%
89	17.033	2536	2541	2551	rVB2	446375	877992	27.14%	1.782%


Sum of corrected areas: 49281579

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020618\
Data File : BF102778.D
Acq On : 6 Feb 2018 12:36
Operator : SJ/JU
Sample : J1454-10DL 4X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
8-SAN-8-EW(4-7)DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

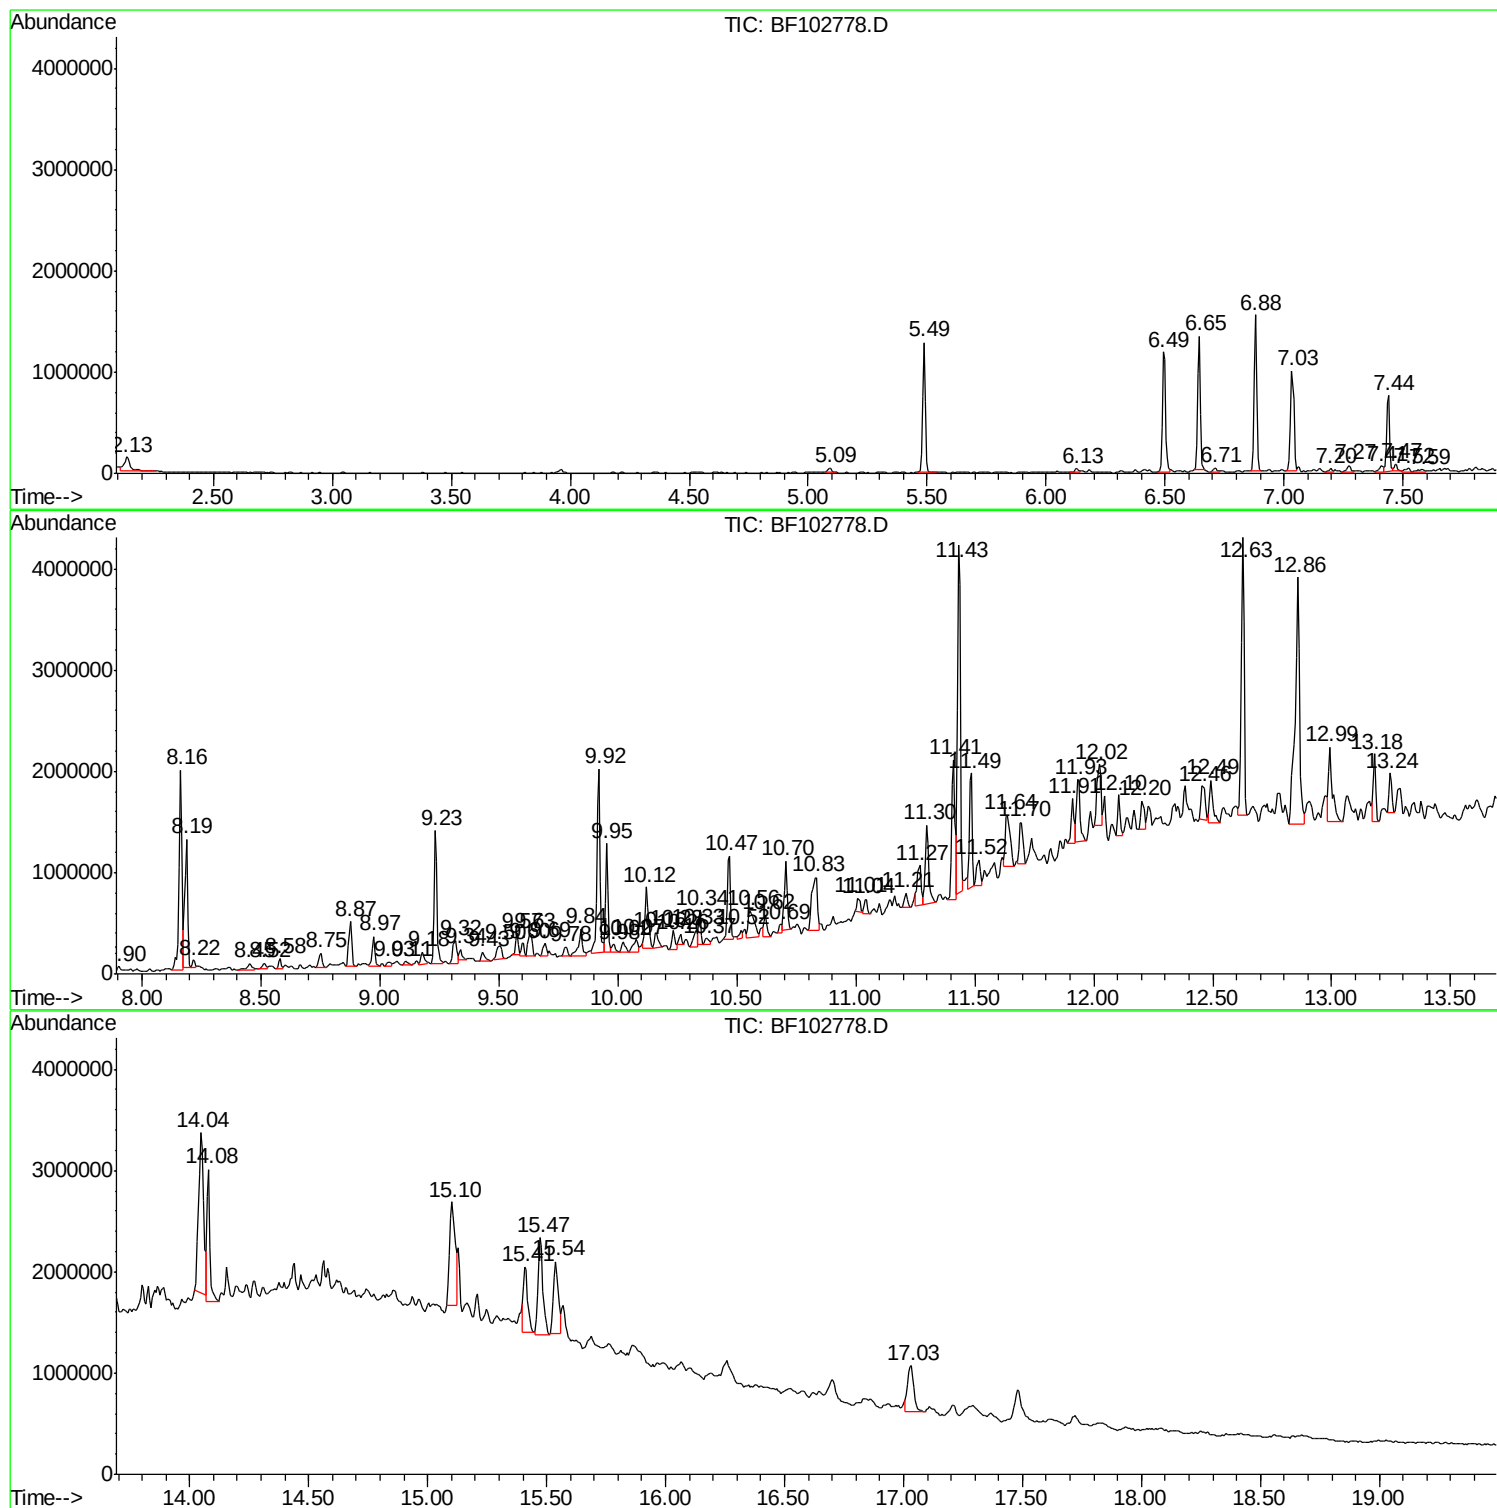

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF020618\
Data_File : BF102778.D
Acq_On : 6_Feb_2018_ 12:366
Operator : SJ/JUU
Sample : J1454-10DL_4XX
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
8-SAN-8-EW(4-7)DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
