


Data Path : Z:\HPCHEM1\BNA F\Data\BF020618\
 Data File : BF102798.D
 Acq On : 6 Feb 2018 22:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

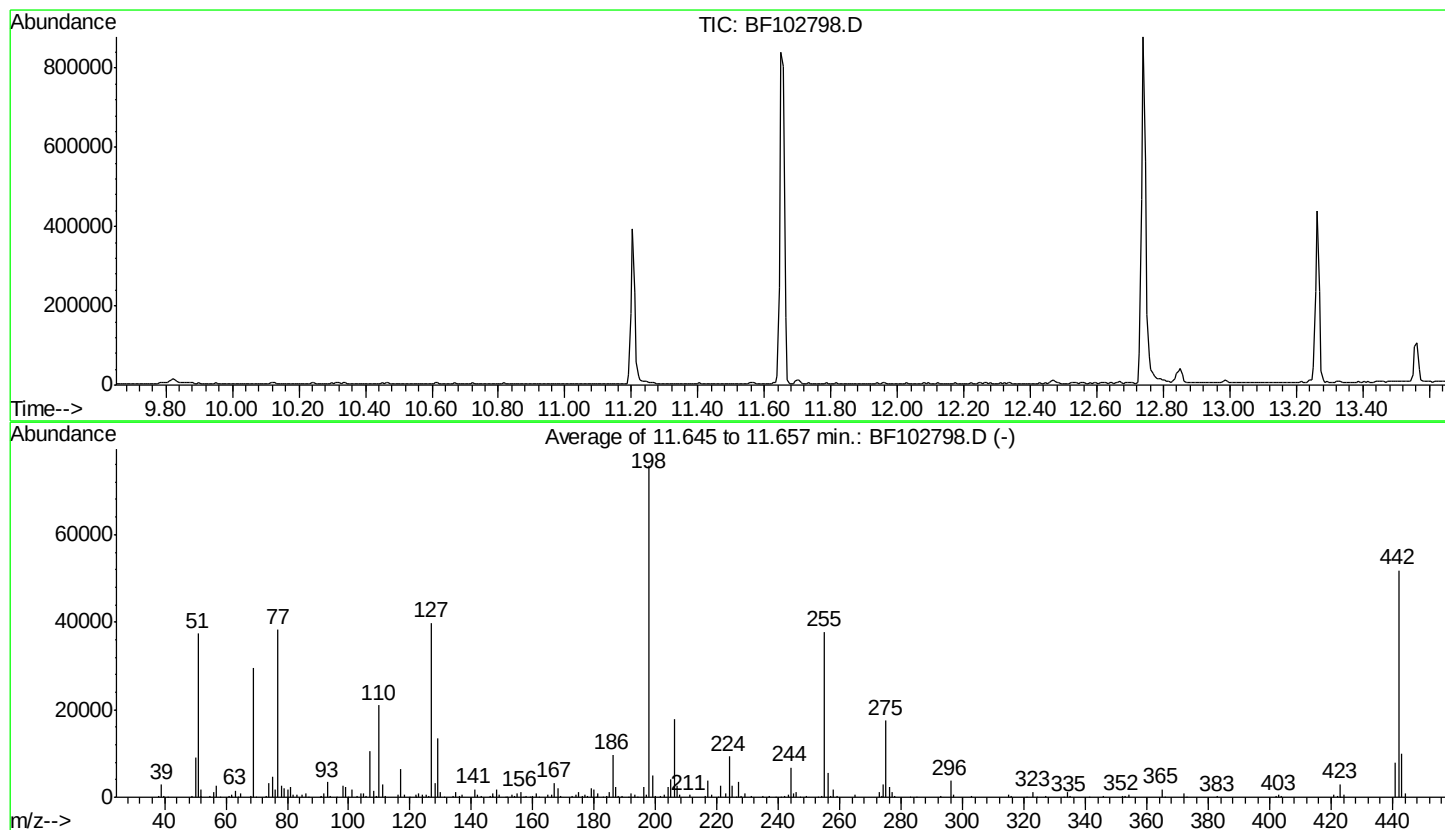

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	37427	PASS
68	69	0.00	2	1.5	446	PASS
69	198	0.00	100	38.8	29410	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	52.6	39816	PASS
197	198	0.00	2	0.9	675	PASS
198	198	100	100	100.0	75746	PASS
199	198	5	9	6.6	4990	PASS
275	198	10	60	23.1	17512	PASS
365	198	1	100	2.4	1788	PASS
441	443	0.01	100	81.2	7994	PASS
442	198	50	100	68.5	51875	PASS
443	442	15	24	19.0	9842	PASS