
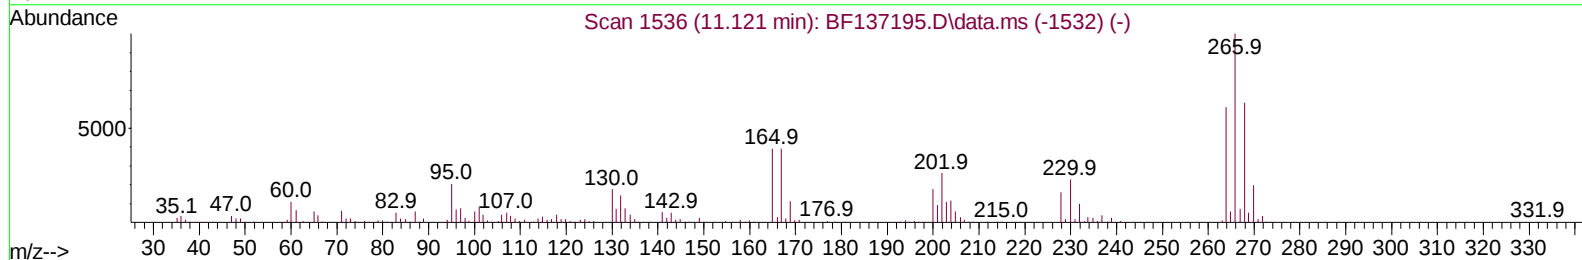
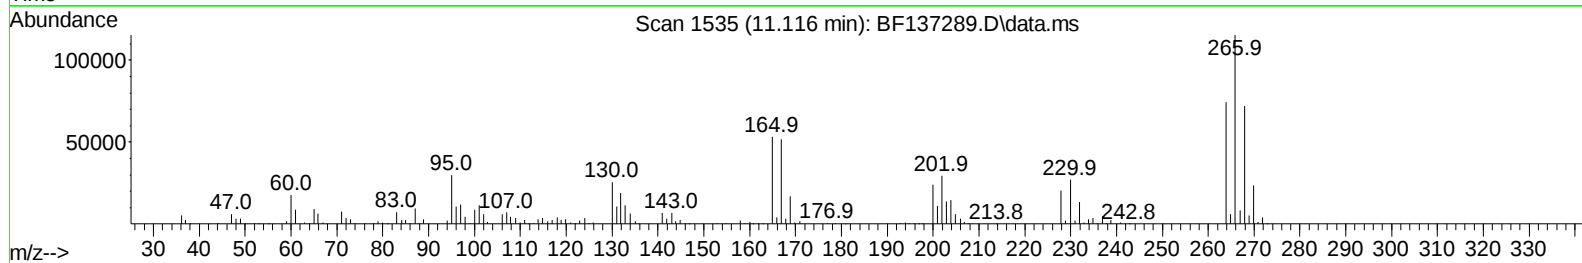


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020624\
Data File : BF137289.D
Acq On : 06 Feb 2024 13:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 05:31:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

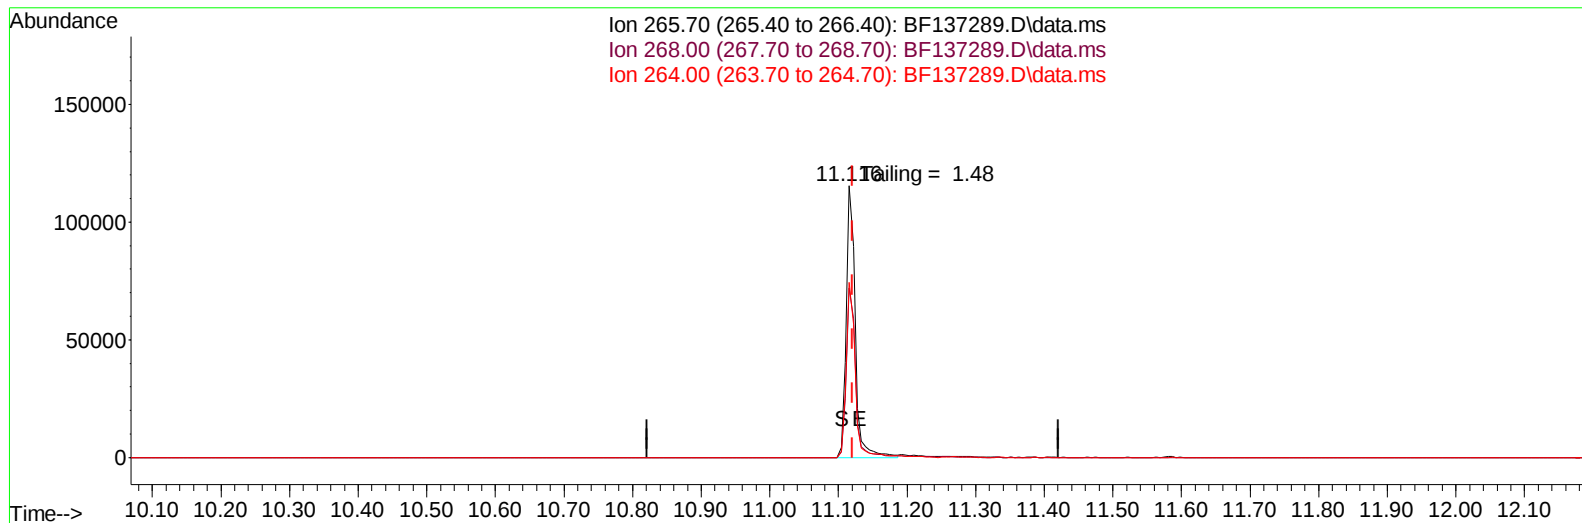

TIC: BF137289.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.005) 36685.33 ng

response 104348

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.29
264.00	61.00	64.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020624\
Data File : BF137289.D
Acq On : 06 Feb 2024 13:25
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 05:31:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

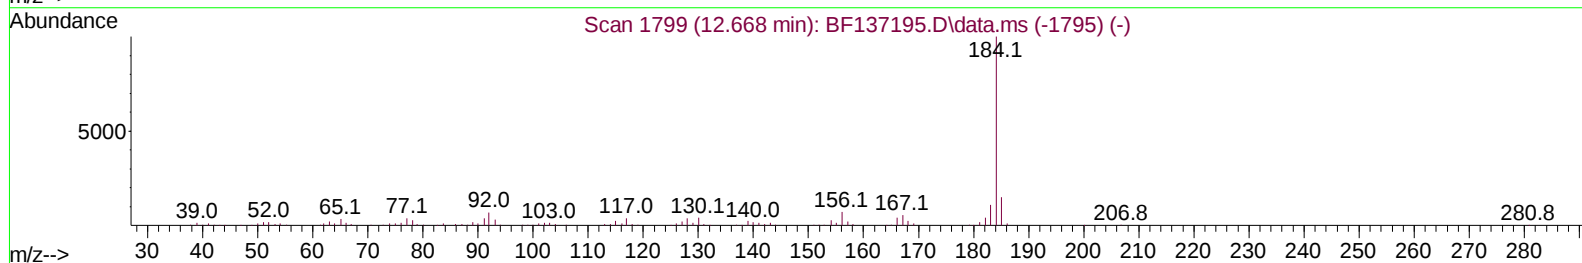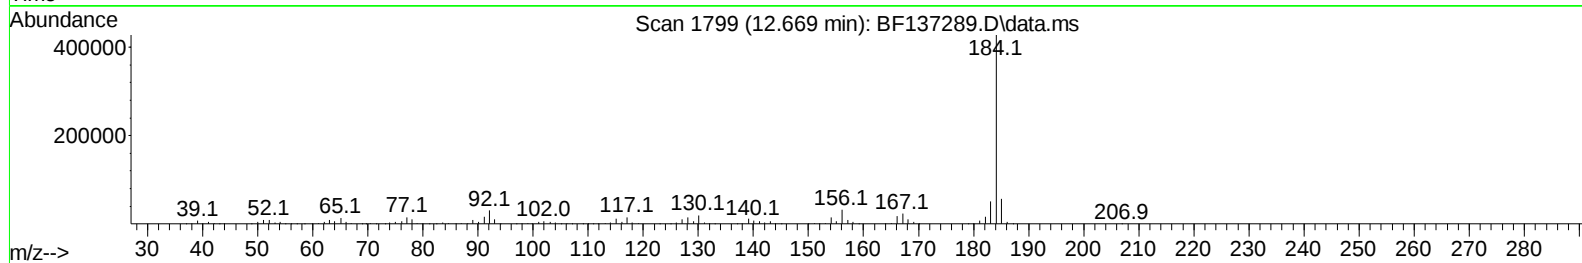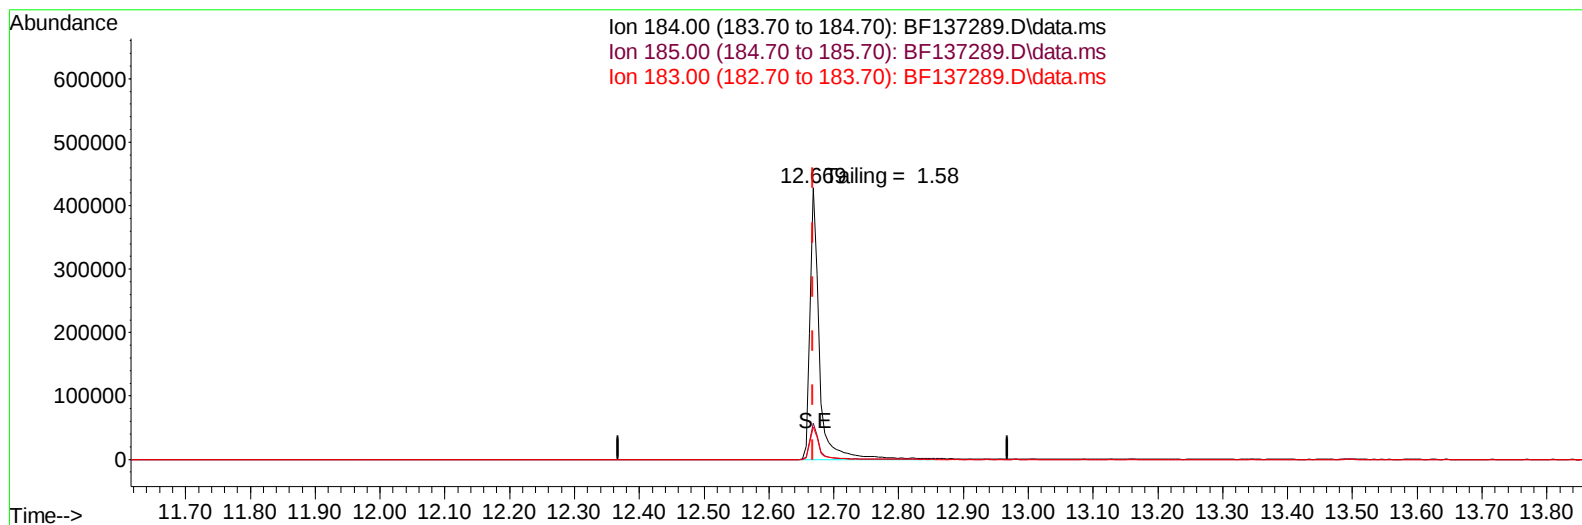

TIC: BF137289.D\data.ms

(77) Benzidine**12.669min (+ 0.001) 0.00 ng****response 437087**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.29
183.00	11.00	12.01
0.00	0.00	0.00