


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020624\
Data File : BF137289.D
Acq On : 06 Feb 2024 13:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 31 04:56:22 2024

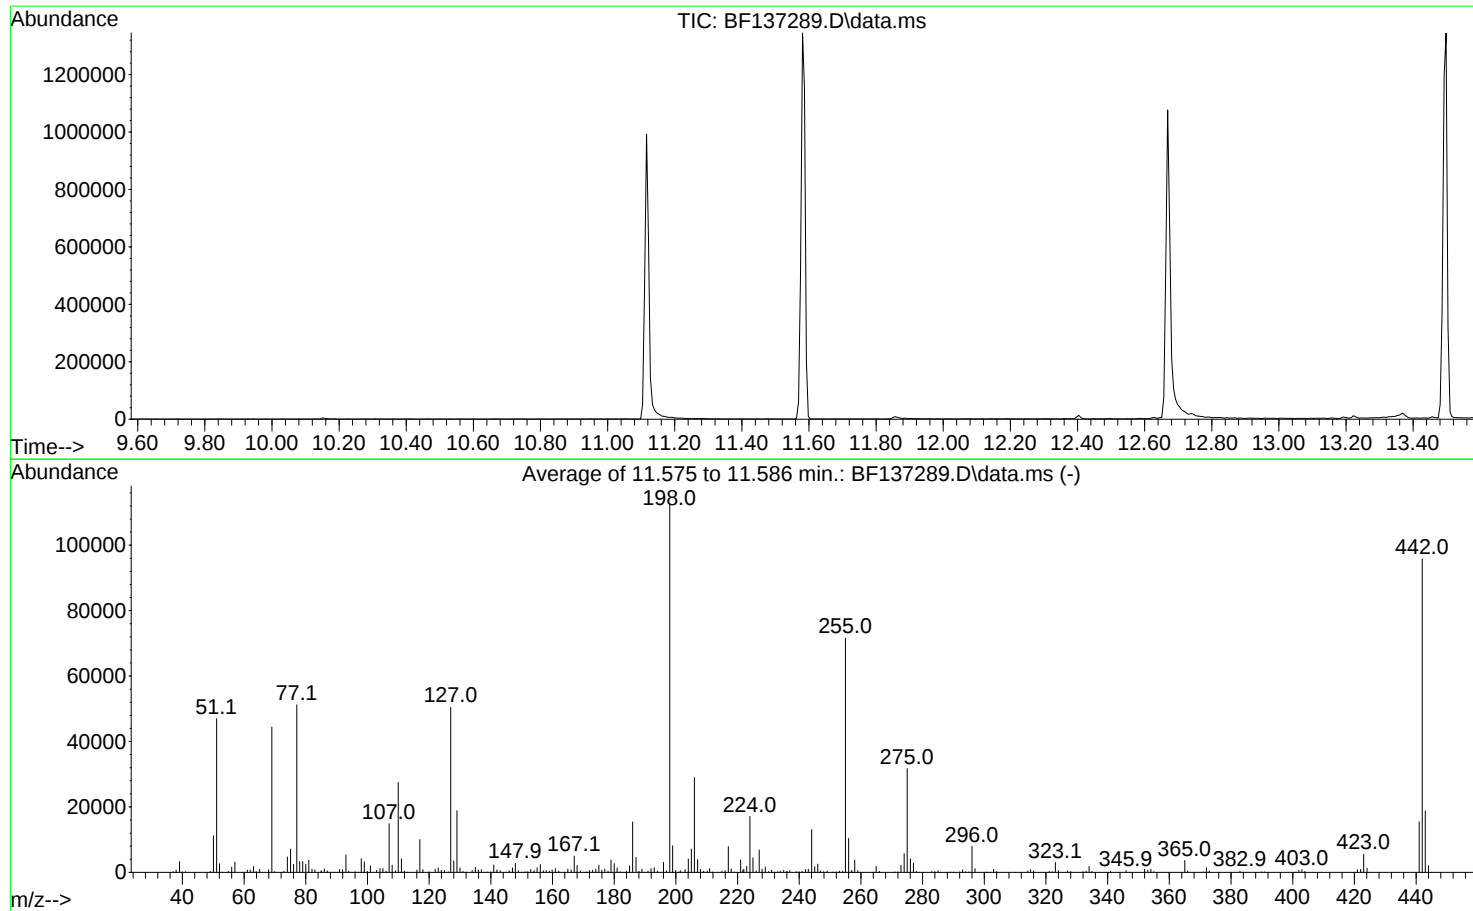

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	41.8	47013	PASS
68	69	0.00	2	1.8	806	PASS
69	198	0.00	100	39.5	44384	PASS
70	69	0.00	2	0.5	225	PASS
127	198	10	80	44.9	50443	PASS
197	198	0.00	2	0.5	506	PASS
198	198	100	100	100.0	112437	PASS
199	198	5	9	7.2	8140	PASS
275	198	10	60	28.2	31706	PASS
365	198	1	100	3.2	3608	PASS
441	198	0.01	100	13.7	15432	PASS
442	442	50	100	100.0	95808	PASS
443	442	15	24	19.6	18772	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2024	BNA_F	<u>BF137289.D</u>
Compound Name	Response	Retention Time
DDT	228705	13.498
DDD	3229	13.222
DDE	54	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3283	231988	1.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020624\
Data File : BF137289.D
Acq On : 06 Feb 2024 13:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 05:31:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

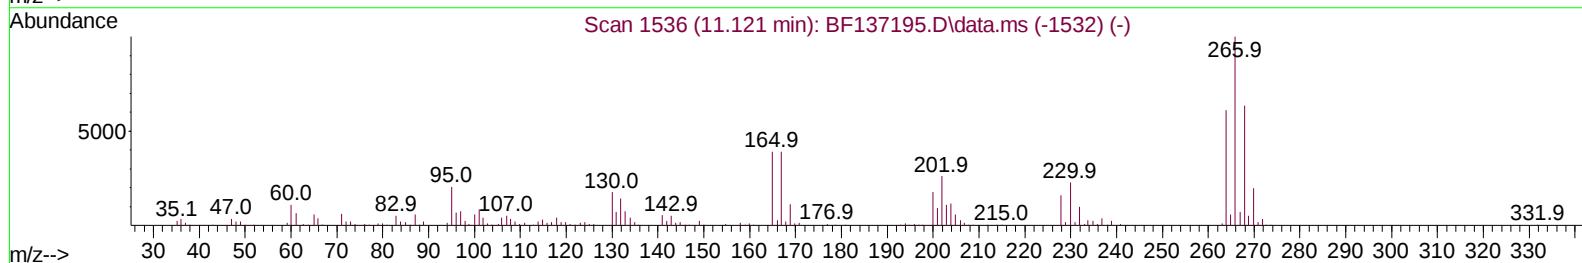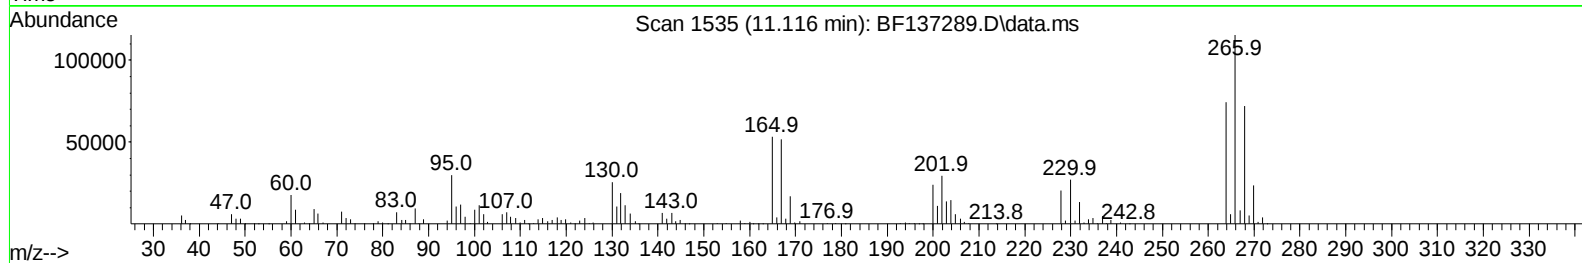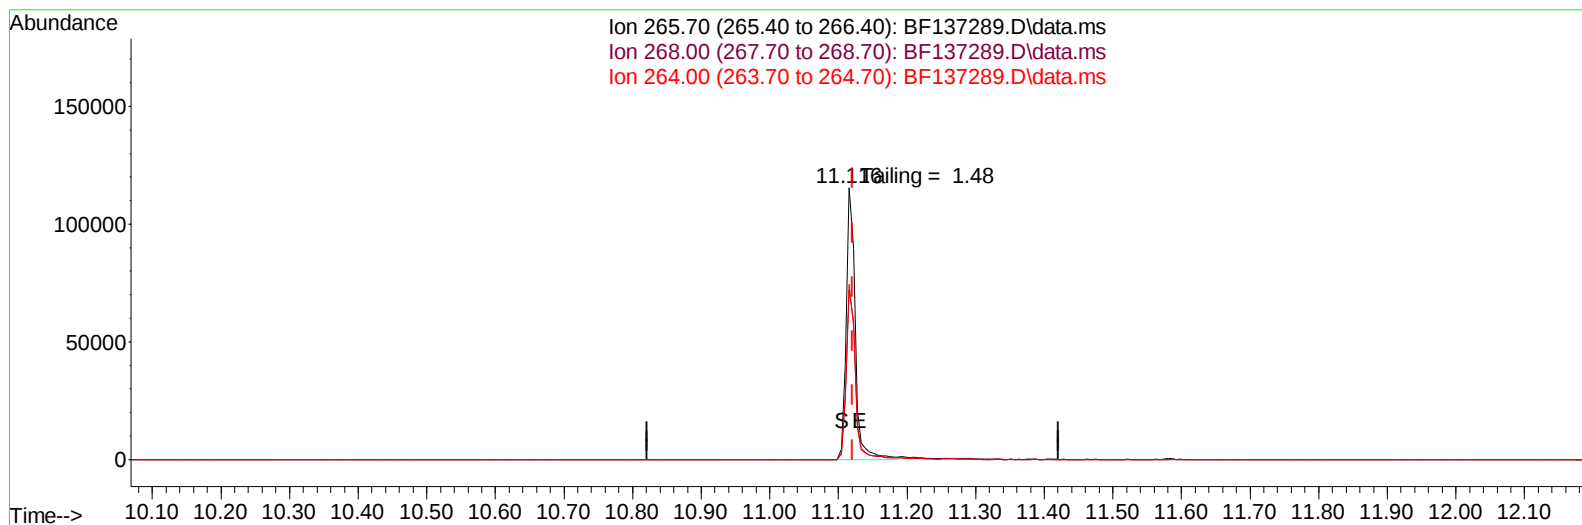

TIC: BF137289.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.005) 36685.33 ng




response 104348

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.29
264.00	61.00	64.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020624\
Data File : BF137289.D
Acq On : 06 Feb 2024 13:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 05:31:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

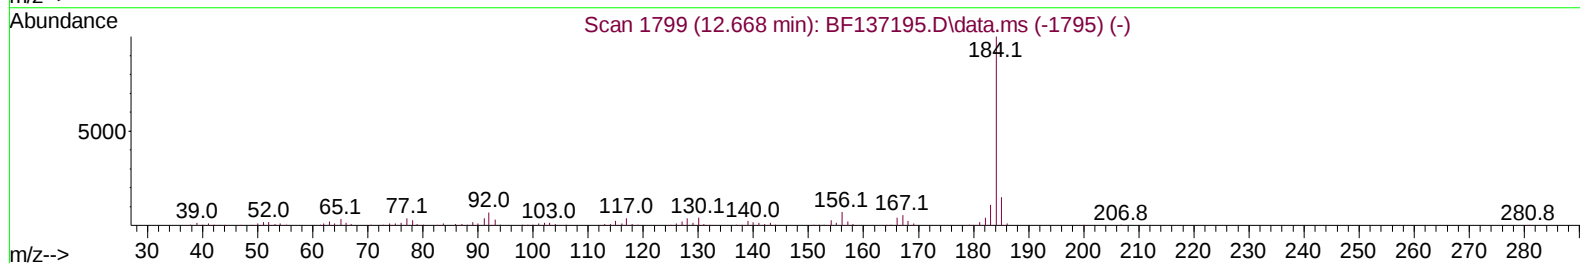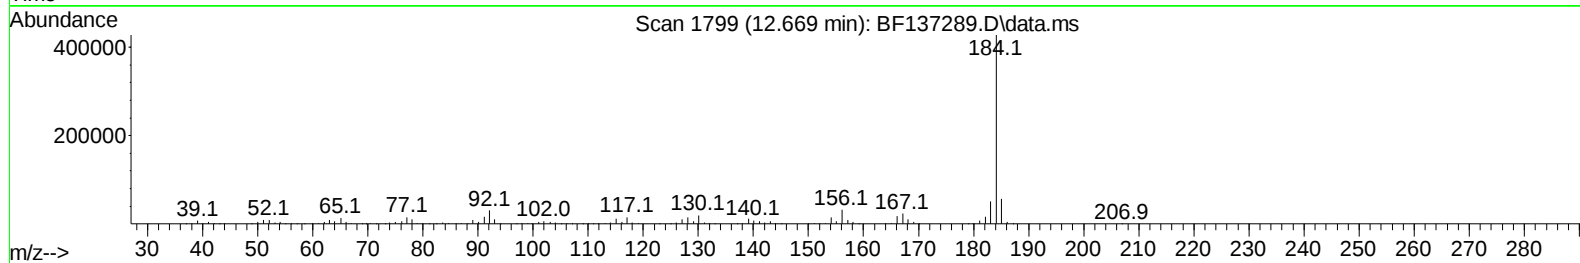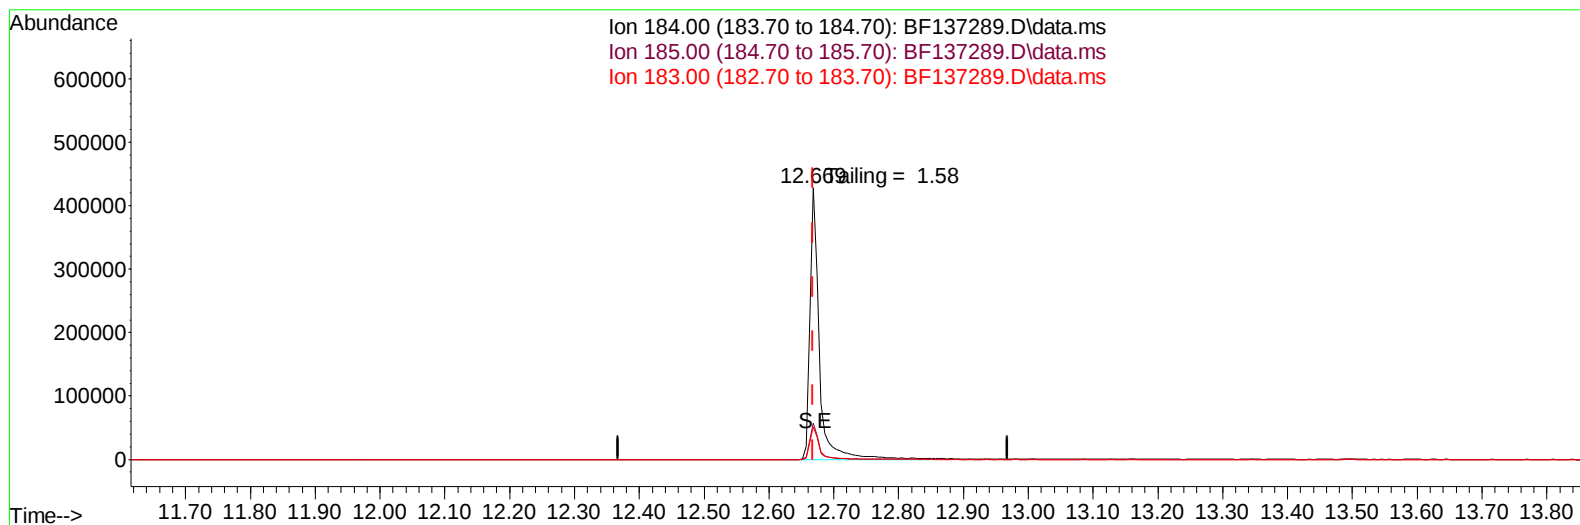

TIC: BF137289.D\data.ms

(77) Benzidine

12.669min (+ 0.001) 0.00 ng

response 437087

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.29
183.00	11.00	12.01
0.00	0.00	0.00