

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
 Data File : BF141485.D
 Acq On : 06 Feb 2025 17:34
 Operator : RC/JU
 Sample : Q1214-01RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PARAMUS-CONDENSATERE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.575	417	422	428	rVB	31594	46000	1.09%	0.221%
2	4.987	488	492	502	rVB	31161	45499	1.08%	0.219%
3	5.369	550	557	560	rBV2	78798	123731	2.93%	0.595%
4	5.410	560	564	583	rVB	682713	912025	21.57%	4.384%
5	6.040	663	671	677	rBV	33699	45783	1.08%	0.220%
6	6.422	731	736	753	rVB	433449	587072	13.88%	2.822%
7	6.787	793	798	804	rBV	435583	535684	12.67%	2.575%
8	7.351	887	894	899	rBV	1592427	2217626	52.44%	10.659%
9	7.669	943	948	957	rBV	42374	59526	1.41%	0.286%
10	8.069	1010	1016	1027	rBV	559647	725418	17.15%	3.487%
11	9.145	1193	1199	1204	rBV	2943160	3895327	92.12%	18.723%
12	9.822	1309	1314	1327	rVB	677677	851197	20.13%	4.091%
13	10.616	1443	1449	1467	rBV	1279413	1736271	41.06%	8.346%
14	11.310	1562	1567	1574	rBV	708312	888886	21.02%	4.273%
15	11.839	1649	1657	1677	rBV2	113960	216325	5.12%	1.040%
16	12.627	1786	1791	1801	rVV	40185	79083	1.87%	0.380%
17	12.716	1801	1806	1816	rVB4	35605	80569	1.91%	0.387%
18	12.904	1831	1838	1843	rBV	3100667	4228669	100.00%	20.326%
19	13.180	1880	1885	1890	rBV	35938	45224	1.07%	0.217%
20	13.469	1925	1934	1944	rVB2	24155	54783	1.30%	0.263%
21	13.622	1955	1960	1969	rVB	42809	57757	1.37%	0.278%
22	13.951	2009	2016	2026	rBV	535174	721906	17.07%	3.470%
23	14.039	2026	2031	2034	rBV	43454	69295	1.64%	0.333%
24	14.227	2053	2063	2067	rBV	28943	72537	1.72%	0.349%
25	14.310	2067	2077	2081	rBV	60853	128189	3.03%	0.616%
26	14.386	2085	2090	2092	rBV	75814	104821	2.48%	0.504%
27	14.463	2100	2103	2107	rVB	153491	191931	4.54%	0.923%
28	14.551	2112	2118	2124	rBV	192813	401949	9.51%	1.932%
29	14.616	2125	2129	2131	rBV	134635	186388	4.41%	0.896%
30	14.692	2138	2142	2146	rBV	211505	282411	6.68%	1.357%
31	14.727	2146	2148	2152	rVB	79201	94188	2.23%	0.453%
32	14.780	2152	2157	2161	rBV	199046	247710	5.86%	1.191%
33	14.816	2161	2163	2168	rVB2	49436	62764	1.48%	0.302%
34	14.869	2168	2172	2179	rVB	115093	163851	3.87%	0.788%
35	15.063	2199	2205	2218	rVB3	24046	74578	1.76%	0.358%
36	15.410	2258	2264	2276	rBV	313376	524257	12.40%	2.520%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141485.D
Acq On : 06 Feb 2025 17:34
Operator : RC/JU
Sample : Q1214-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARAMUS-CONDENSATERE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.962	2522	2528	2544	rVB7	12301	45340	1.07%	0.218%
----	--------	------	------	------	------	-------	-------	-------	--------




Sum of corrected areas: 20804570

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141485.D
Acq On : 06 Feb 2025 17:34
Operator : RC/JU
Sample : Q1214-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARAMUS-CONDENSATERE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

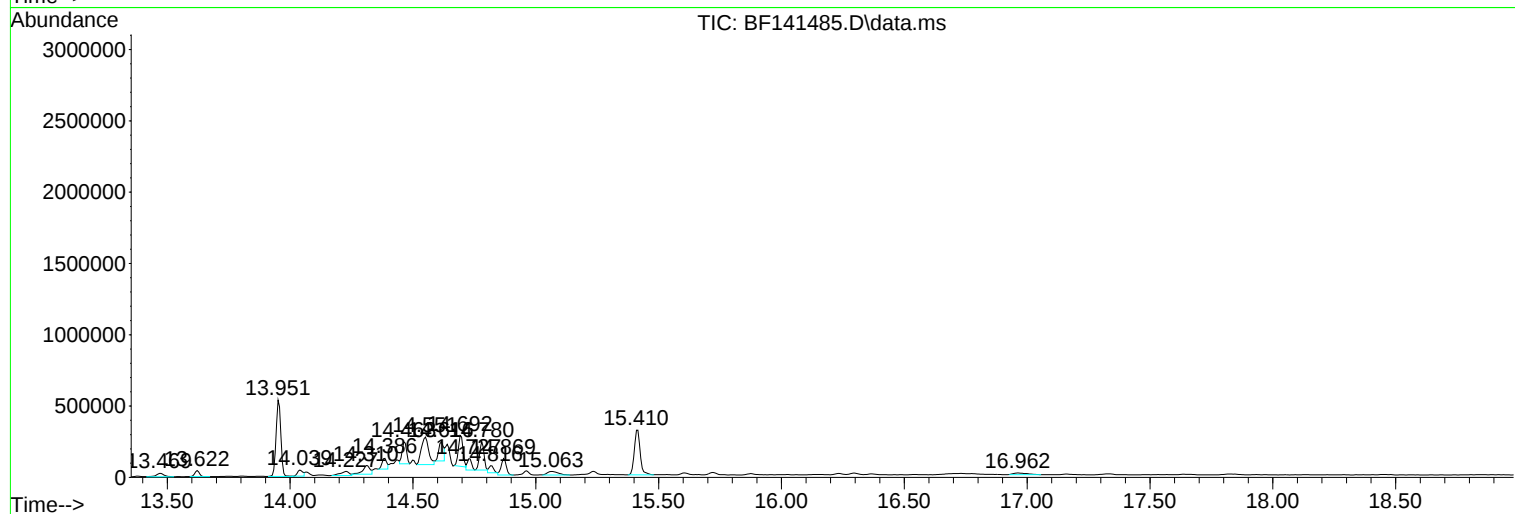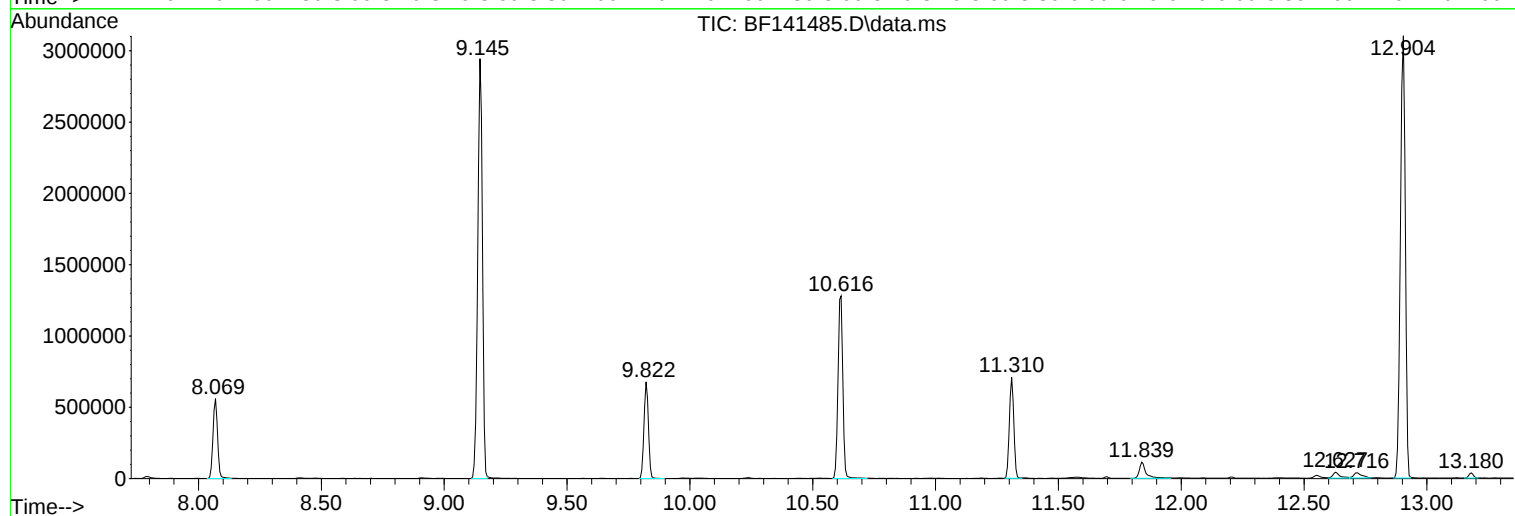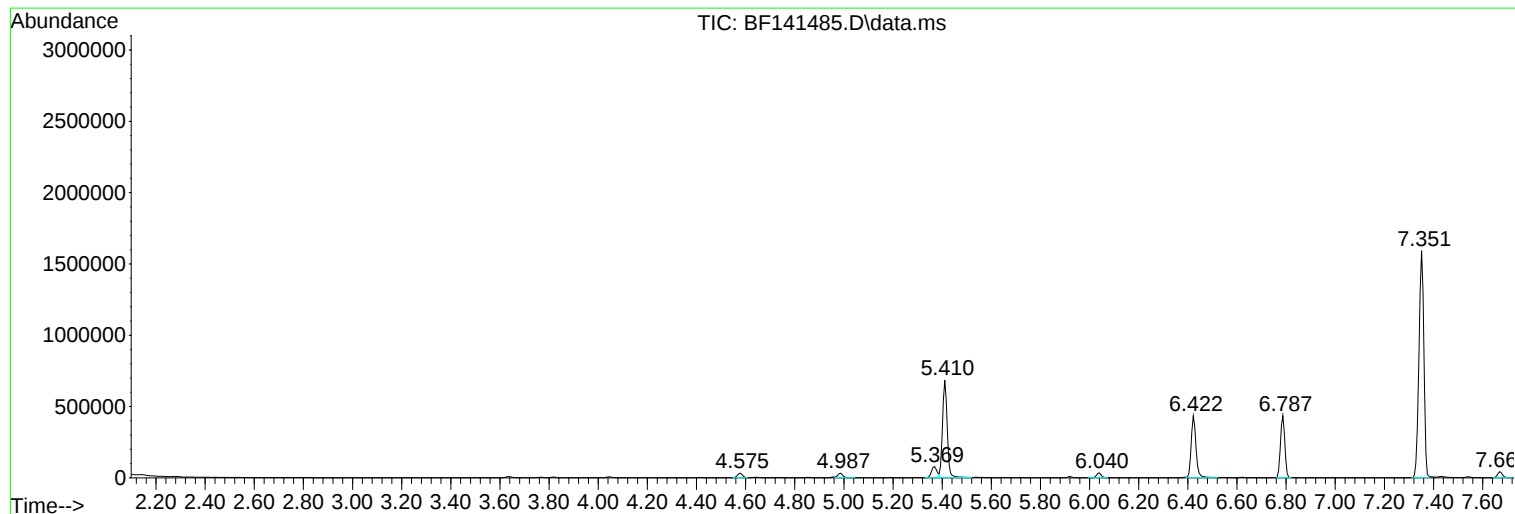

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141485.D
Acq On : 06 Feb 2025 17:34
Operator : RC/JU
Sample : Q1214-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARAMUS-CONDENSATERE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141485.D
Acq On : 06 Feb 2025 17:34
Operator : RC/JU
Sample : Q1214-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARAMUS-CONDENSATERE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------