
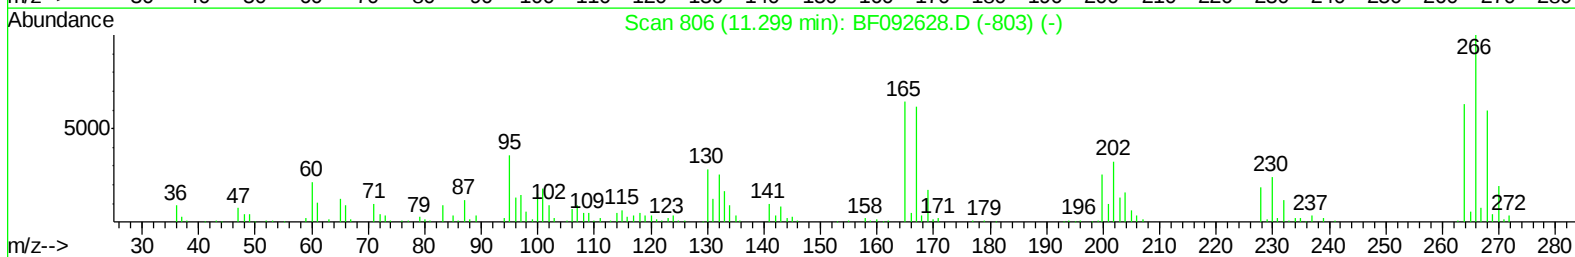
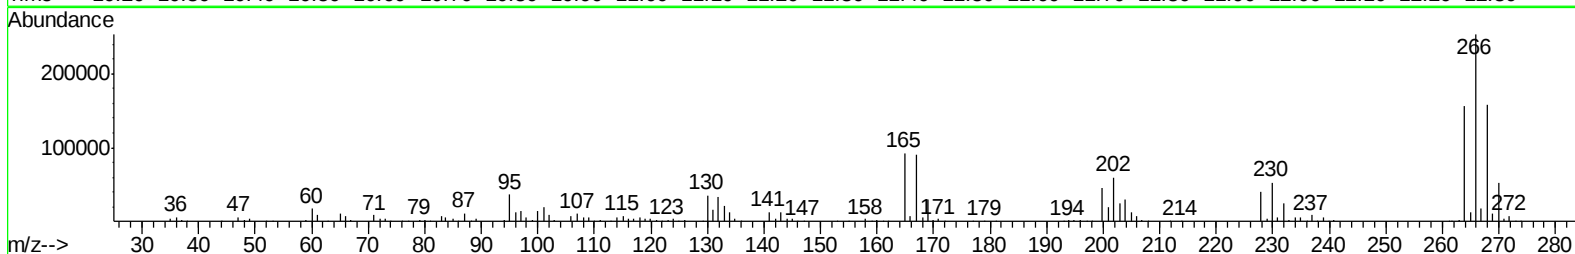


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020717\
Data File : BF092822.D
Acq On : 7 Feb 2017 11:34
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:04:53 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 23:52:21 2017
Response via : Initial Calibration

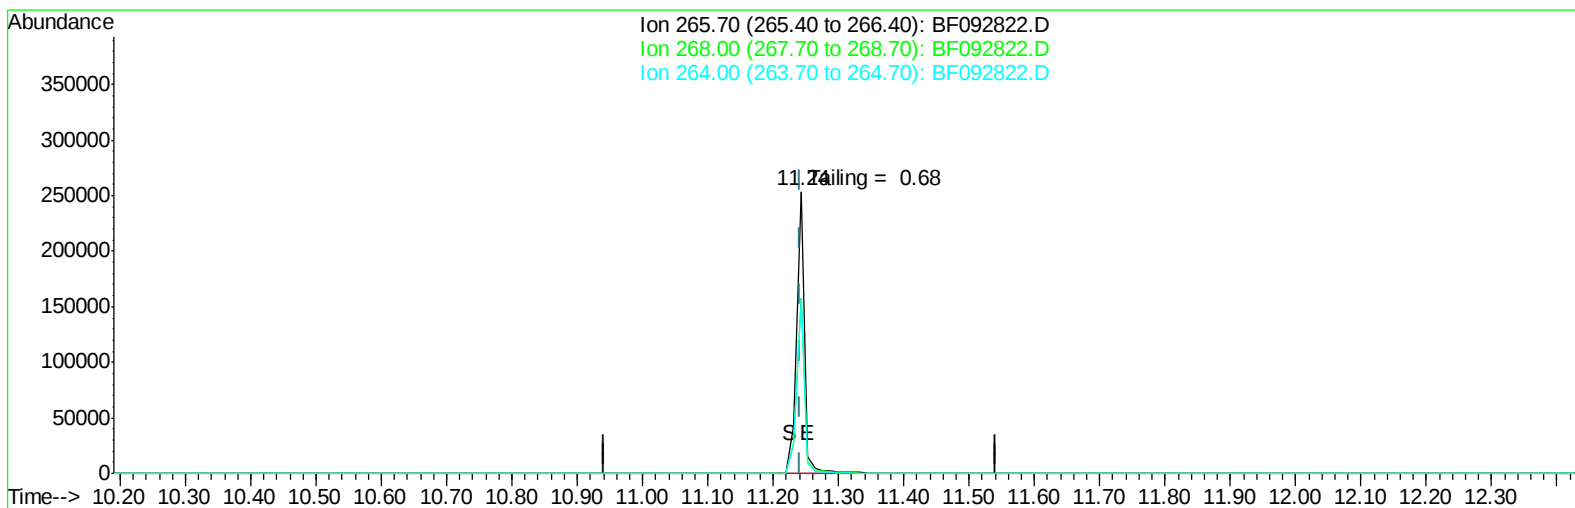

TIC: BF092822.D

(69) Pentachlorophenol (C)




11.242min (-0.000) 0.00ng

response 225917

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.51
264.00	62.90	61.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020717\
 Data File : BF092822.D
 Acq On : 7 Feb 2017 11:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:04:53 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 07 23:52:21 2017
 Response via : Initial Calibration

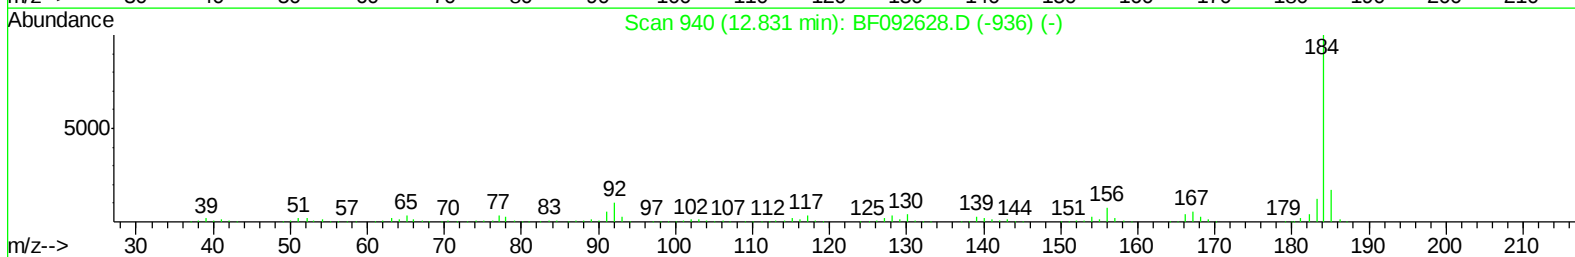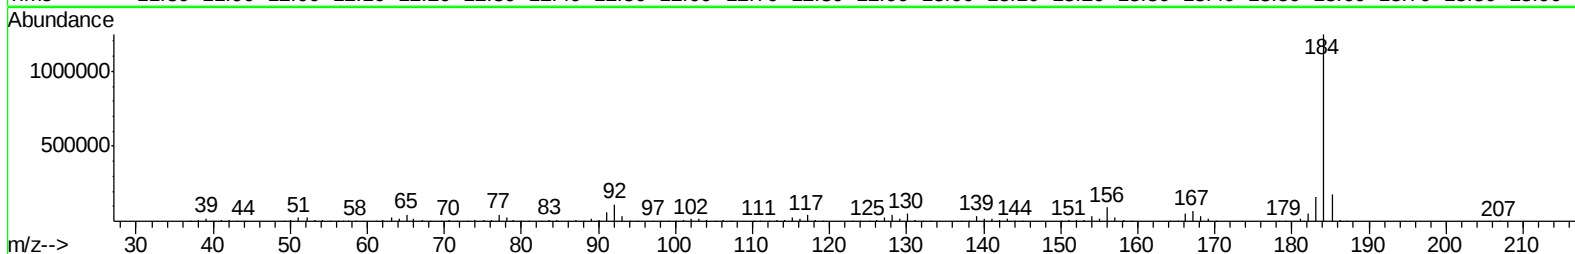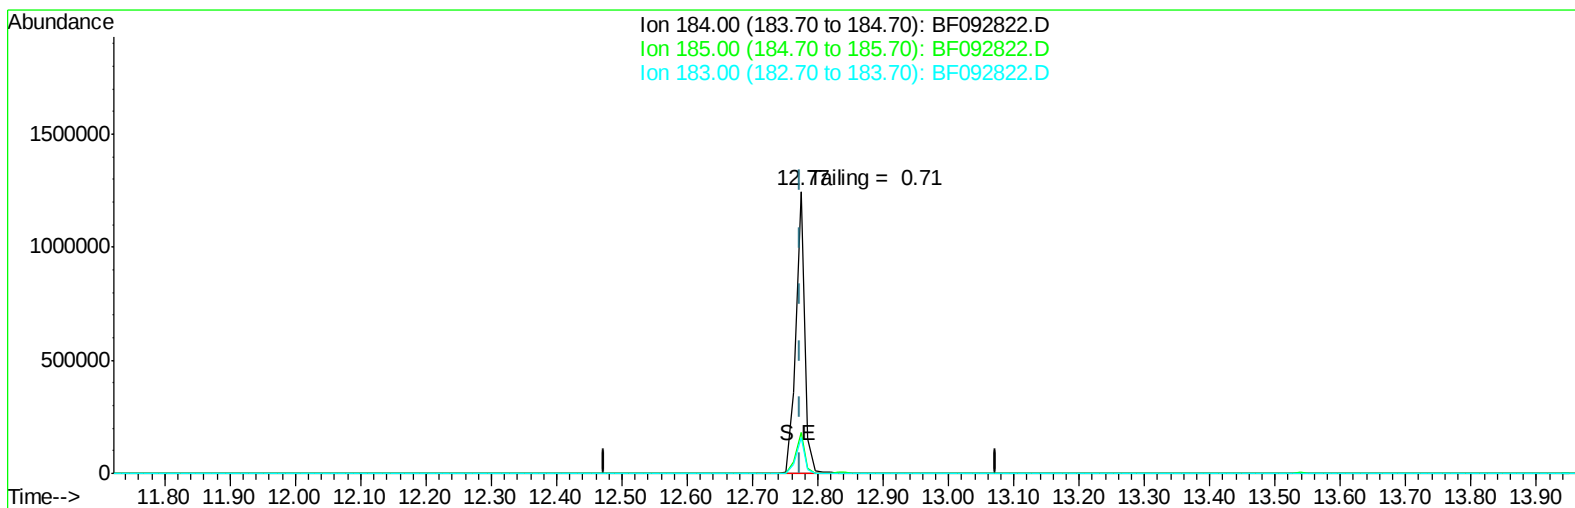

TIC: BF092822.D

(76) Benzidine

12.773min (-0.000) 73569.47ng

response 1232053

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.36
183.00	11.50	12.82
0.00	0.00	0.00