
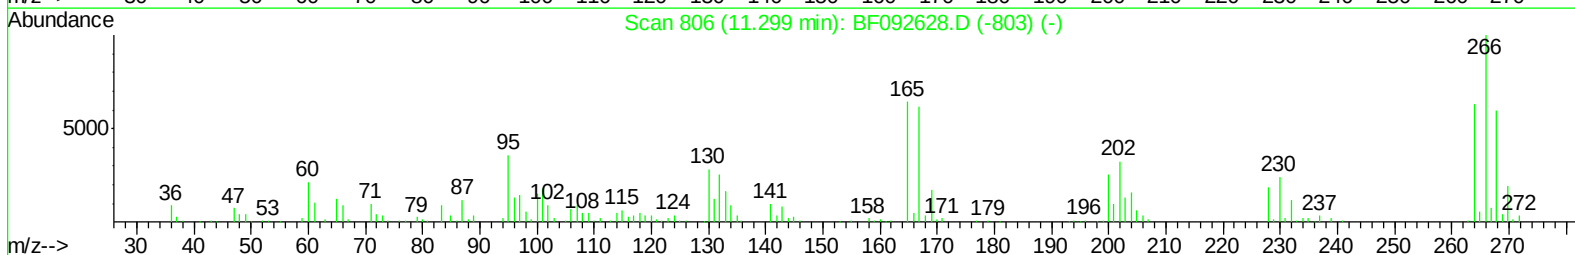
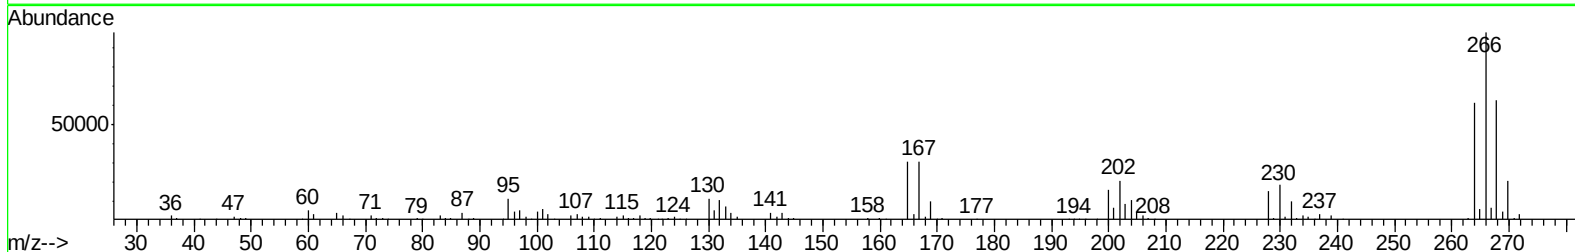


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020717\
Data File : BF092845.D
Acq On : 8 Feb 2017 00:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:05:36 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 23:52:21 2017
Response via : Initial Calibration

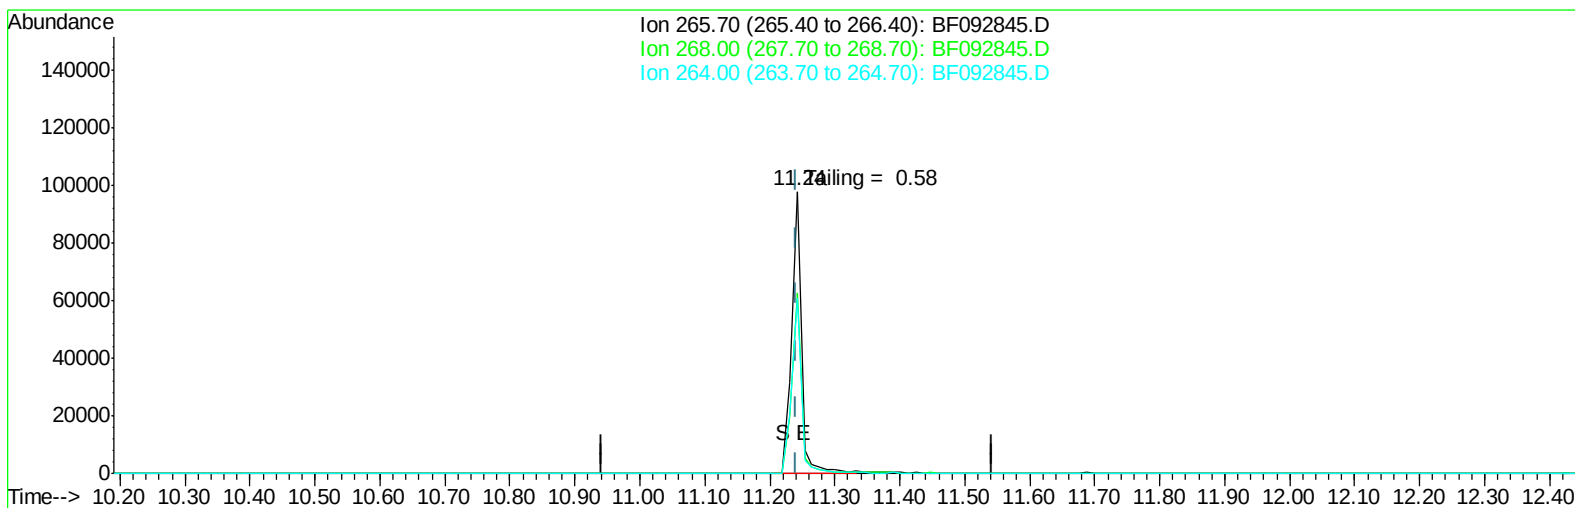

TIC: BF092845.D

(69) Pentachlorophenol (C)




11.242min (-0.000) 0.00ng

response 103129

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.16
264.00	62.90	62.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020717\
Data File : BF092845.D
Acq On : 8 Feb 2017 00:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:05:36 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 23:52:21 2017
Response via : Initial Calibration

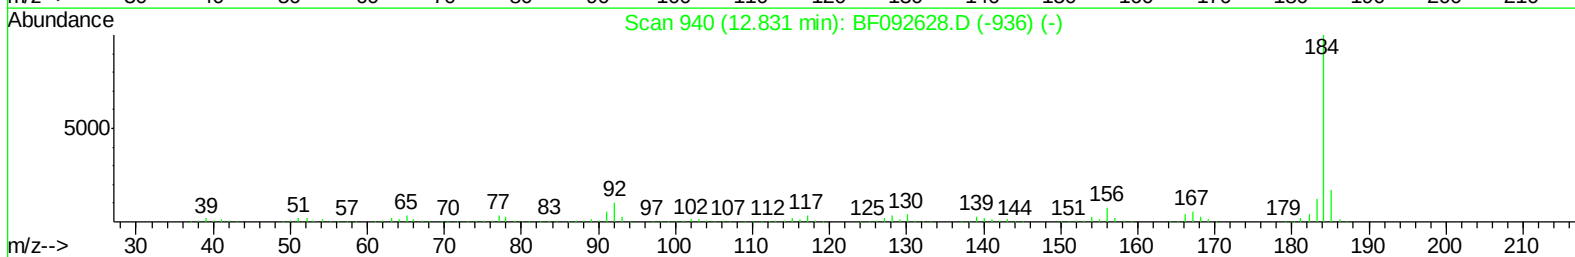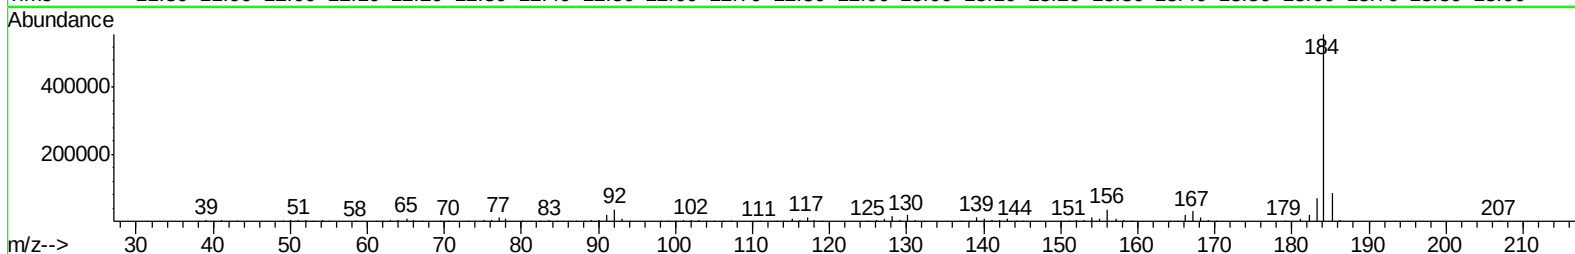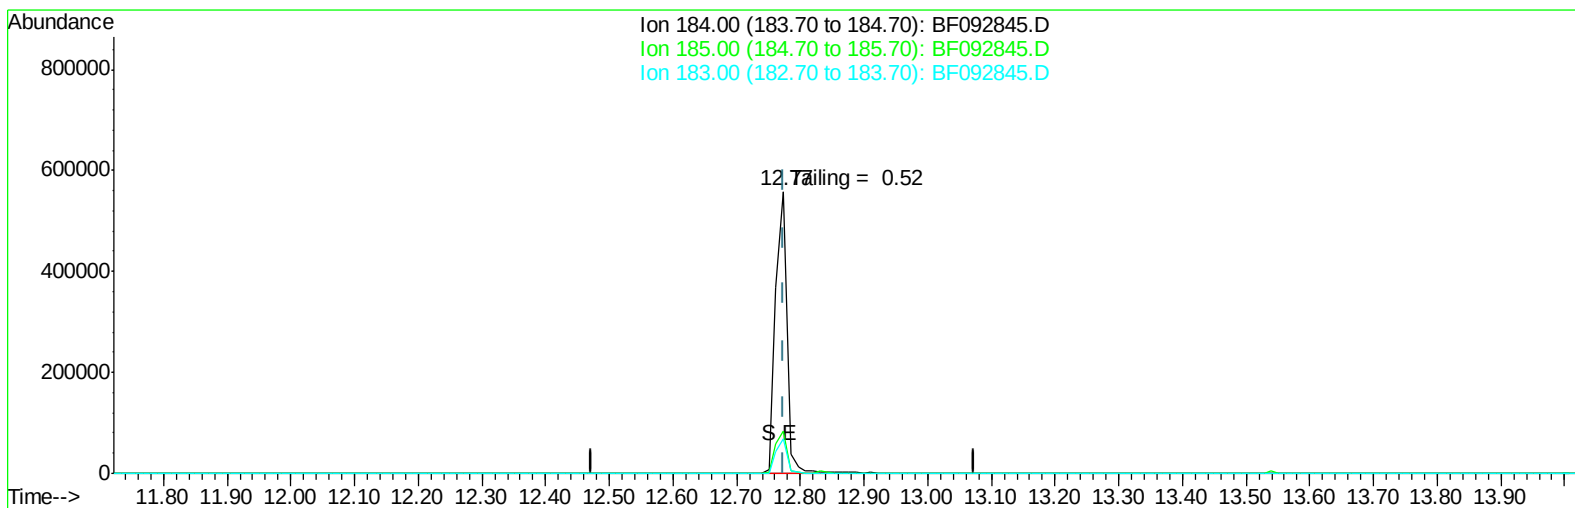

TIC: BF092845.D

(76) Benzidine

12.774min (-0.000) 0.00ng

response 698470

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.05
183.00	11.50	12.28
0.00	0.00	0.00