


Data Path : Z:\HPCHEM1\BNA F\Data\BF020717\
 Data File : BF092822.D
 Acq On : 7 Feb 2017 11:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

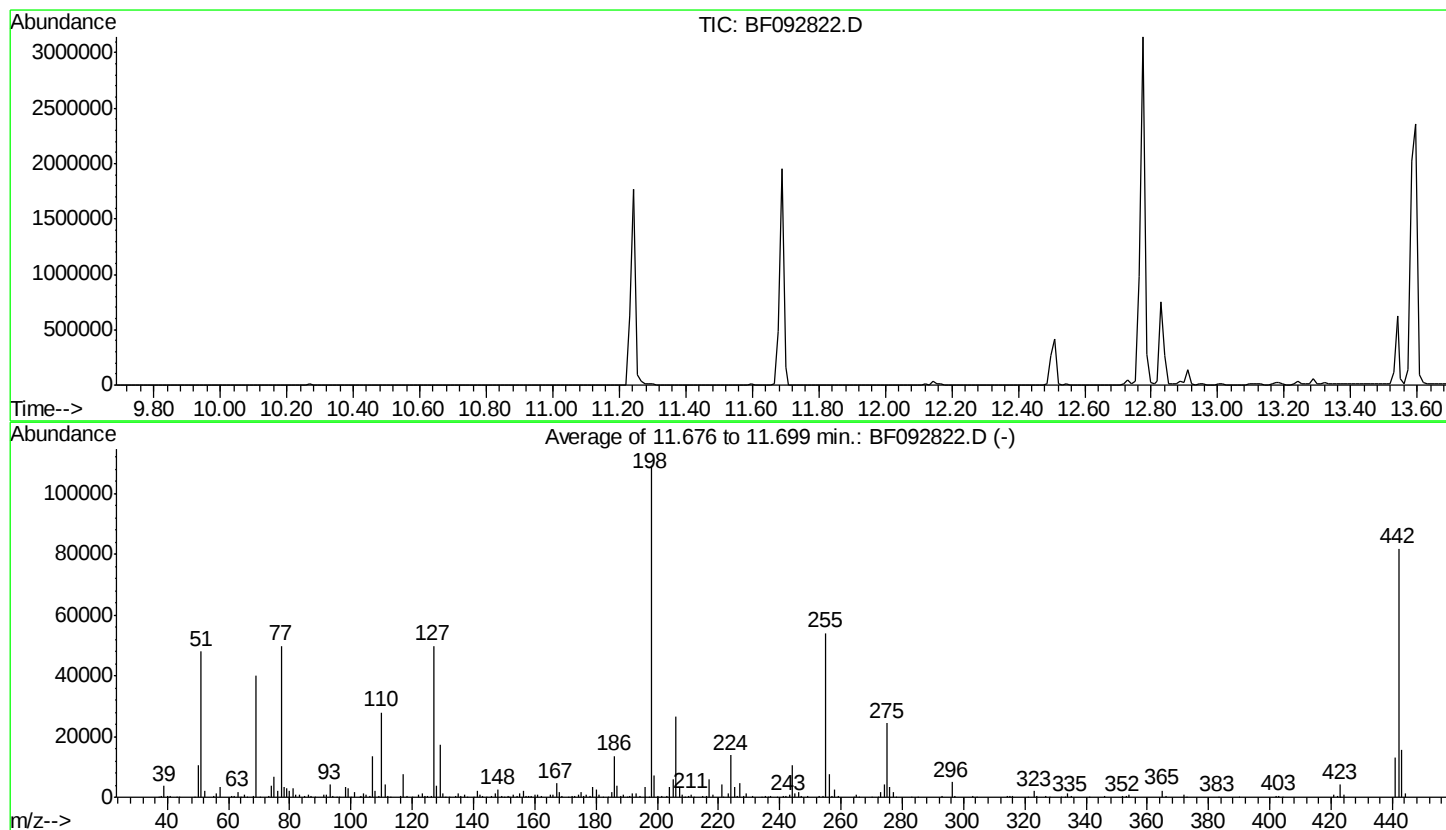

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	47907	PASS
68	69	0.00	2	1.6	638	PASS
69	198	0.00	100	36.7	40078	PASS
70	69	0.00	2	0.3	116	PASS
127	198	10	80	45.6	49734	PASS
197	198	0.00	2	0.2	196	PASS
198	198	100	100	100.0	109077	PASS
199	198	5	9	6.7	7255	PASS
275	198	10	60	22.3	24305	PASS
365	198	1	100	2.0	2204	PASS
441	442	0.01	24	15.9	13020	PASS
442	198	50	100	75.0	81794	PASS
443	442	15	24	19.2	15701	PASS