


Data Path : Z:\HPCHEM1\BNA F\Data\BF020717\
 Data File : BF092845.D
 Acq On : 8 Feb 2017 00:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

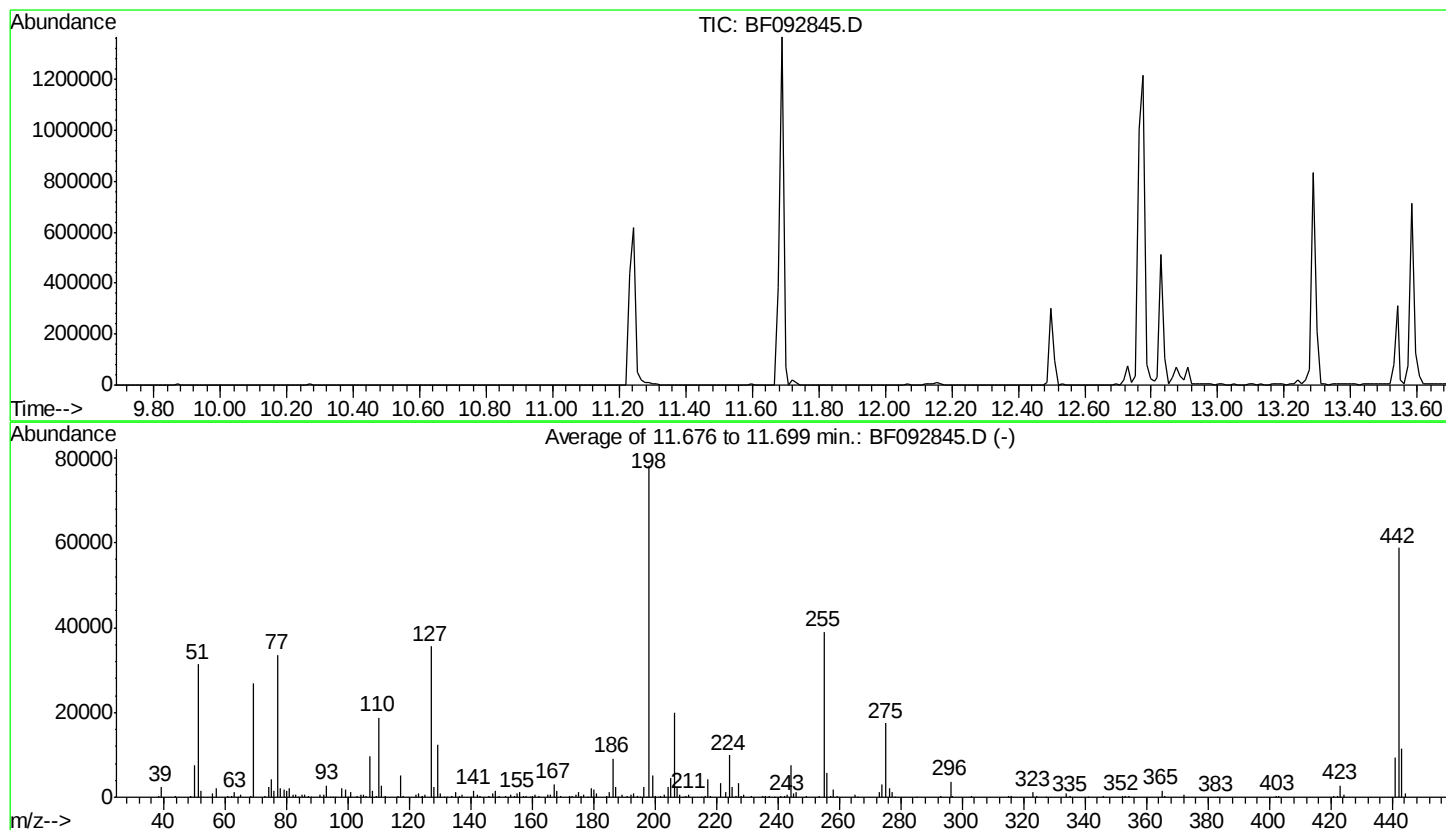

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	31293	PASS
68	69	0.00	2	1.7	454	PASS
69	198	0.00	100	34.3	26825	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.5	35543	PASS
197	198	0.00	2	0.2	148	PASS
198	198	100	100	100.0	78189	PASS
199	198	5	9	6.7	5246	PASS
275	198	10	60	22.2	17393	PASS
365	198	1	100	2.0	1556	PASS
441	442	0.01	24	15.7	9224	PASS
442	198	50	100	75.1	58744	PASS
443	442	15	24	19.7	11545	PASS