

Data Path : U:\HPCHEM1\BNA F\DATA\BF020718\
 Data File : BF102810.D
 Acq On : 7 Feb 2018 12:53
 Operator : SJ/JU
 Sample : PB106327BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Feb 08 01:31:06 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 12:44:16 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	170727	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	711133	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	330056	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	586439	20.00	ng	0.00
75) Chrysene-d12	14.04	240	449887	20.00	ng	0.00
86) Perylene-d12	15.52	264	350316	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	639580	56.89	ng	0.00
7) Phenol-d6	6.50	99	789566	58.33	ng	0.00
23) Nitrobenzene-d5	7.44	82	493360	48.13	ng	-0.01
41) 2,4,6-Tribromophenol	10.70	330	164564	61.95	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	925970	46.55	ng	-0.01
78) Terphenyl-d14	12.99	244	896417	47.18	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.44	70	66784	7.483	ng	# 80
25) Isophorone	7.44	82	493354	20.900	ng	# 64
32) Benzoic acid	8.16	122	137	8.562	ng	# 1
47) 2-Nitroaniline	9.63	65	874	3.592	ng	# 1
49) Dimethylphthalate	9.63	163	69167	2.688	ng	100
50) 2,6-Dinitrotoluene	9.92	165	42313	8.642	ng	# 25
56) 2,4-Dinitrotoluene	9.92	165	42313	9.106	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.70	198	401	8.944	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF020718\
Data File : BF102810.D
Acq On : 7 Feb 2018 12:53
Operator : SJ/JU
Sample : PB106327BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 08 01:31:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

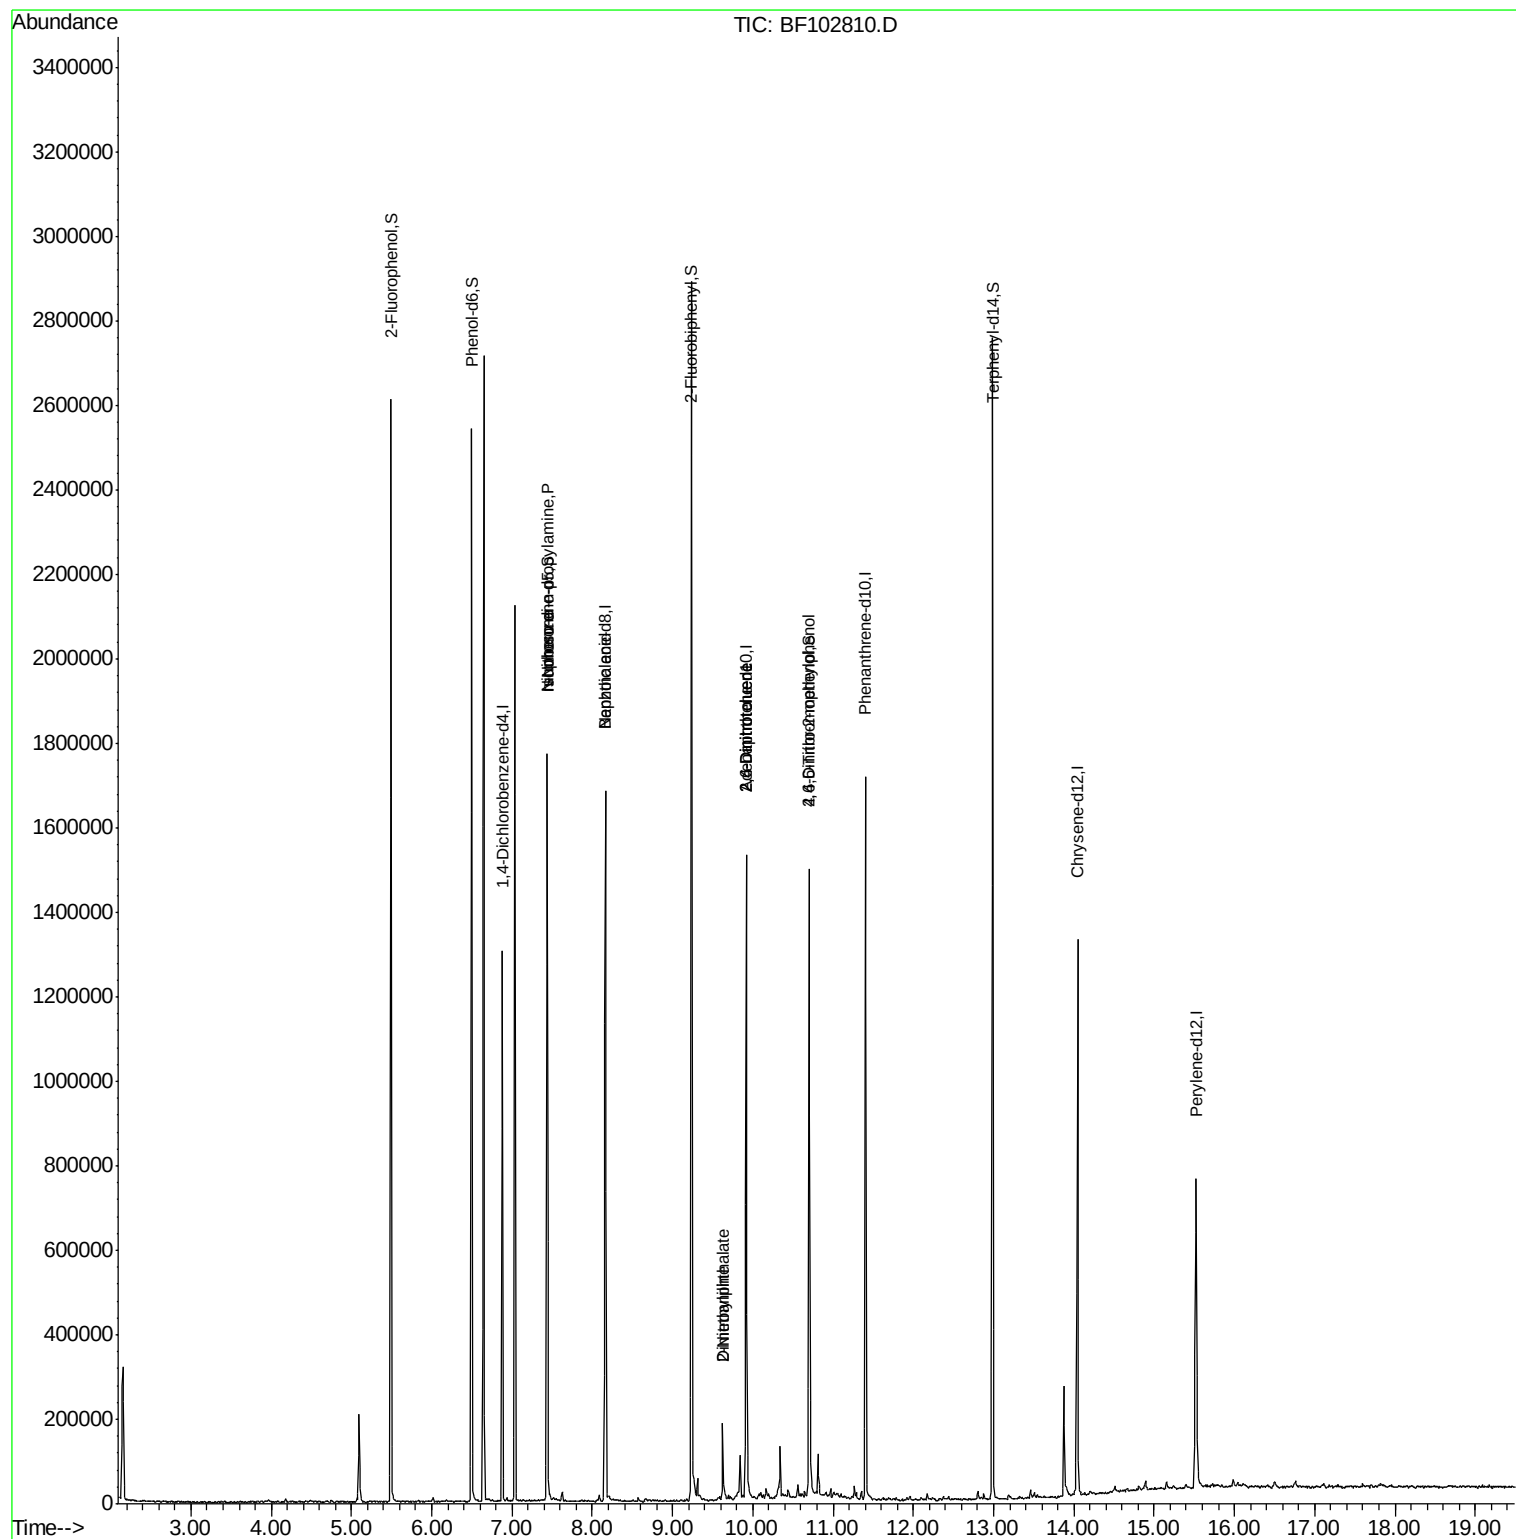

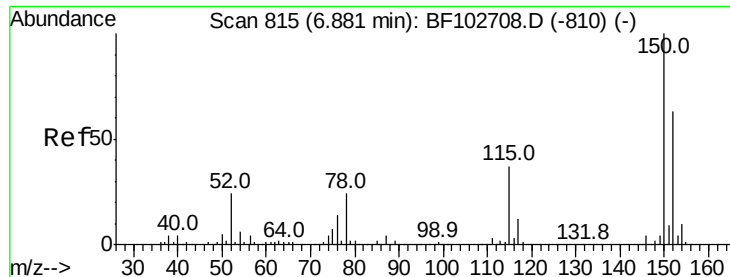


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. 0.00 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.5	124.6	186.8
115	60.4	50.1	75.1

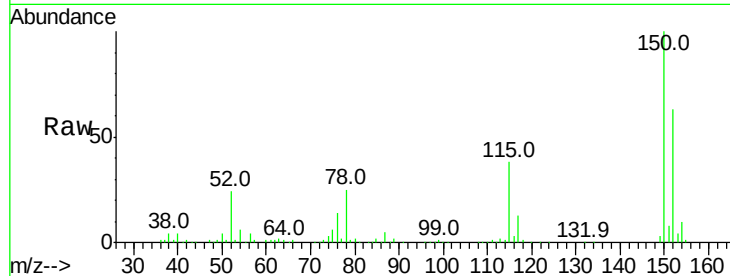


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

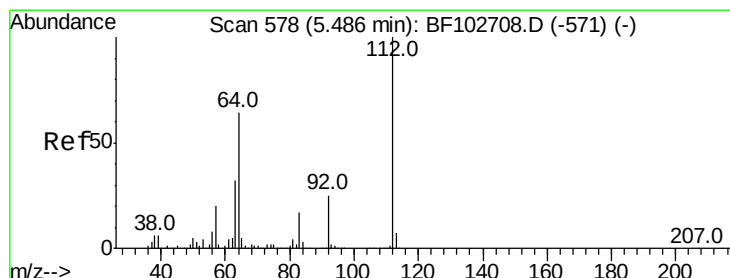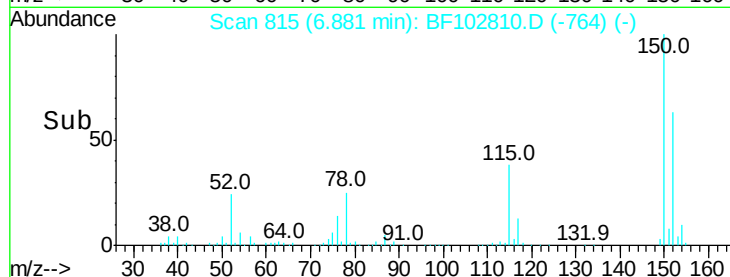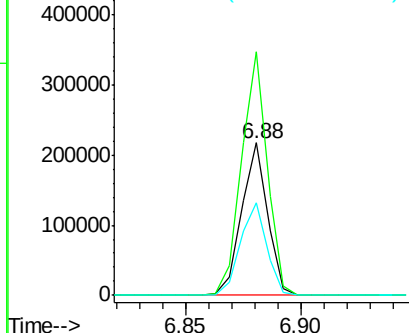



#5


2-Fluorophenol
Concen: 56.893 ng
RT: 5.49 min Scan# 579
Delta R.T. 0.00 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.9	47.9	71.9
63	32.2	23.7	35.5

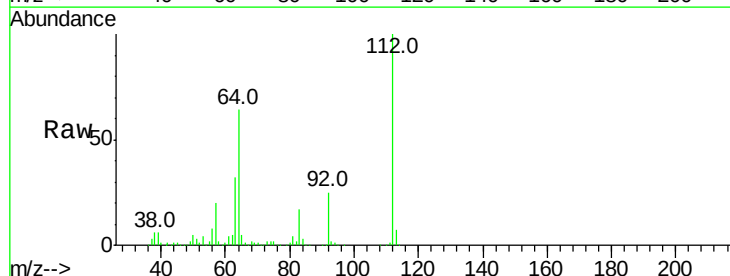

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

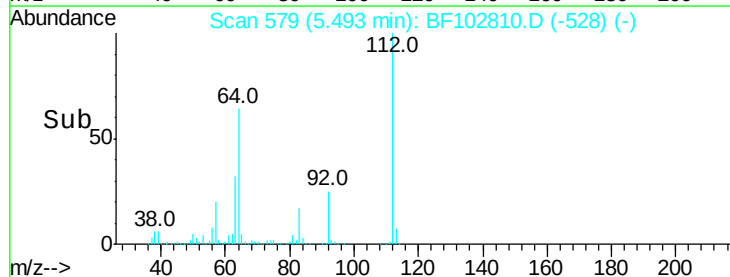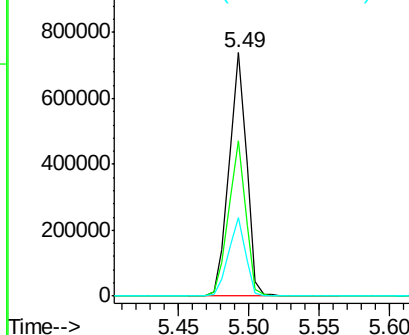

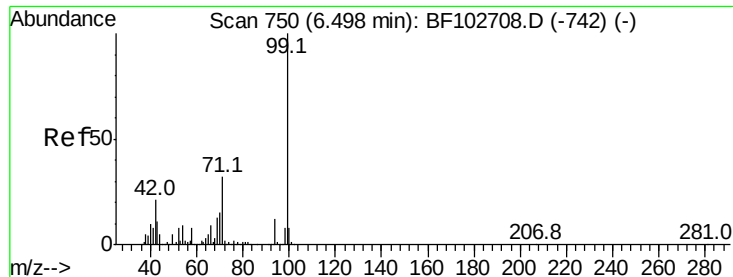

#7

Phenol-d6

Concen: 58.331 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.01 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53

Instrument :

BNA_F

ClientSampled :





Tot Ion: 99 Resp: 789566

Ion Ratio Lower Upper

99 100

42 19.6 14.5 21.7

71 32.3 25.4 38.0

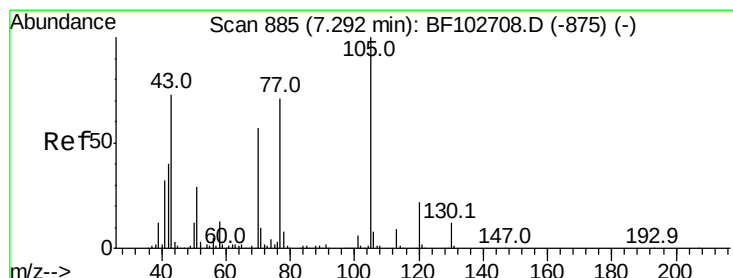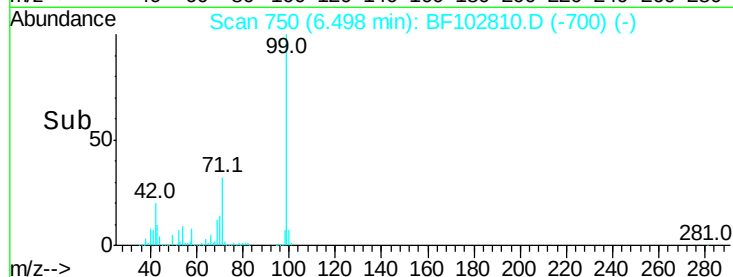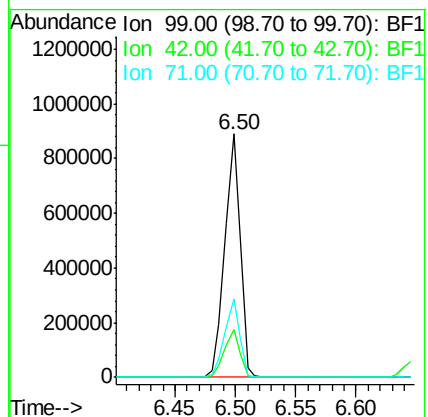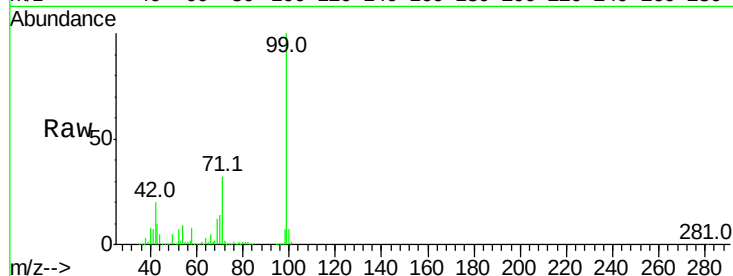

#19

n-Nitroso-di-n-propylamine

Concen: 7.483 ng

RT: 7.44 min Scan# 910

Delta R.T. 0.14 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53

Tgt Ion: 70 Resp: 66784




Ion Ratio Lower Upper


70 100

42 50.2 47.5 71.3

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#

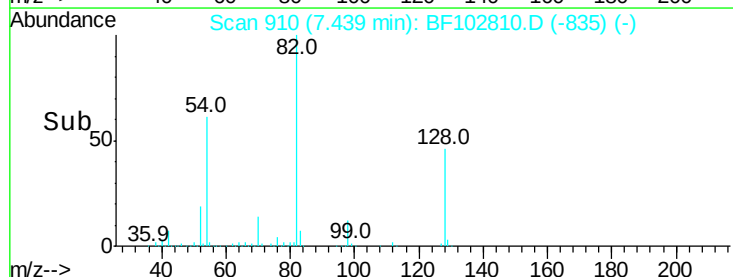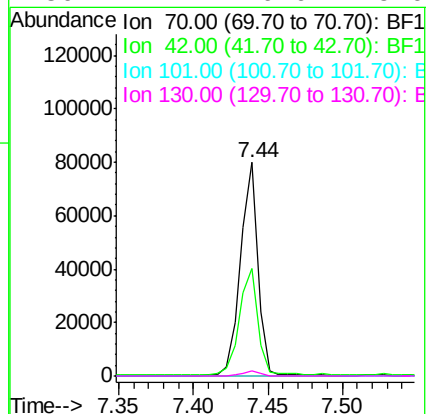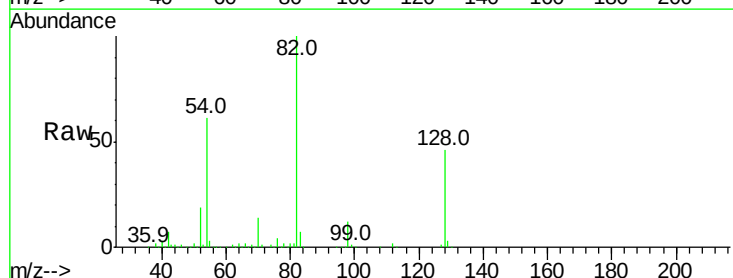







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.16 min Scan# 1033
Delta R.T. -0.01 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	711133
Ion Ratio	Lower	Upper
136	100	
137	11.5	8.9 13.3
54	9.6	6.6 9.8
68	6.3	5.0 7.4

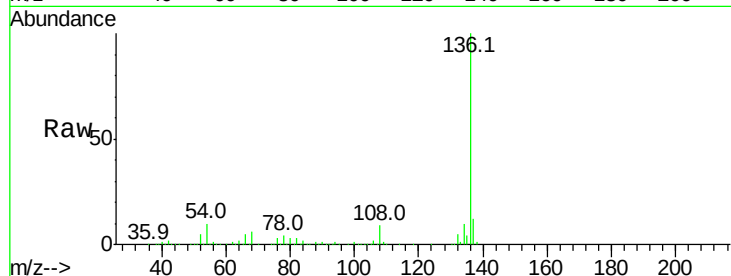


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1


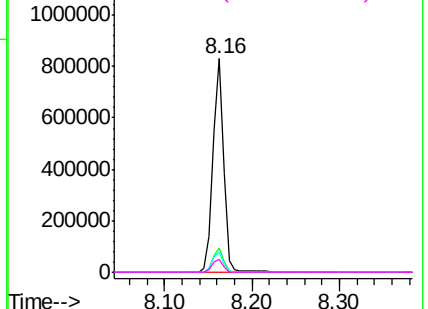



#23
Nitrobenzene-d5
Concen: 48.127 ng
RT: 7.44 min Scan# 910
Delta R.T. -0.01 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Tgt Ion: 82	Resp:	493360
Ion Ratio	Lower	Upper
82	100	
128	46.2	36.1 54.1
54	61.0	41.4 62.2

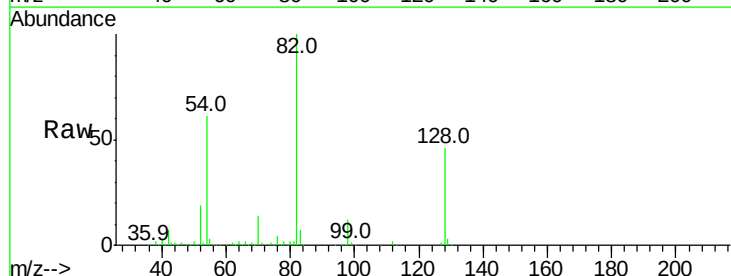

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

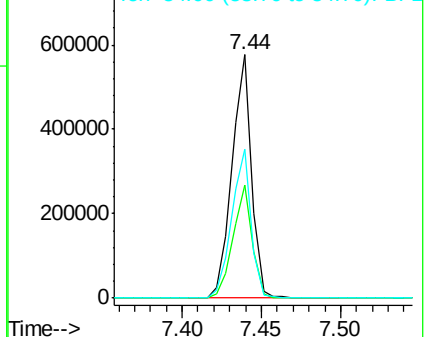



#25

Isophorone

Concen: 20.900 ng

RT: 7.44 min Scan# 910

Delta R.T. -0.26 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 82 Resp: 493354

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

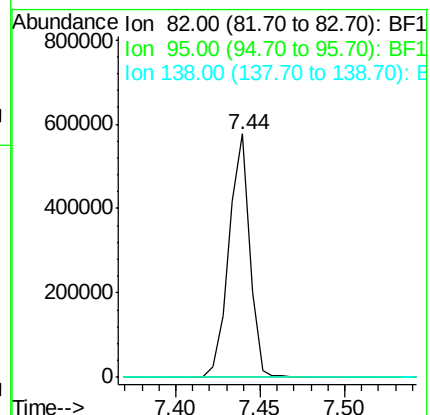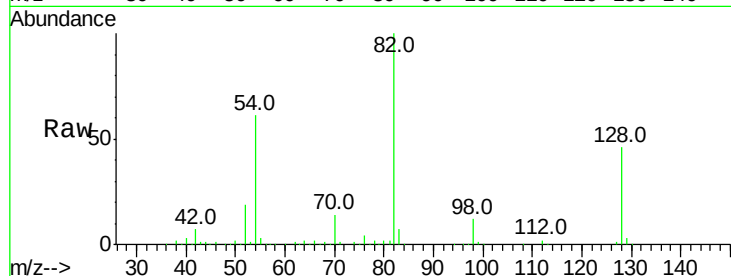

#32

Benzoic acid

Concen: 8.562 ng

RT: 8.16 min Scan# 1032

Delta R.T. 0.22 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53




Tgt Ion:122 Resp: 137


Ion Ratio Lower Upper

122 100

105 105.9 101.1 141.1

77 393.1 70.7 110.7#

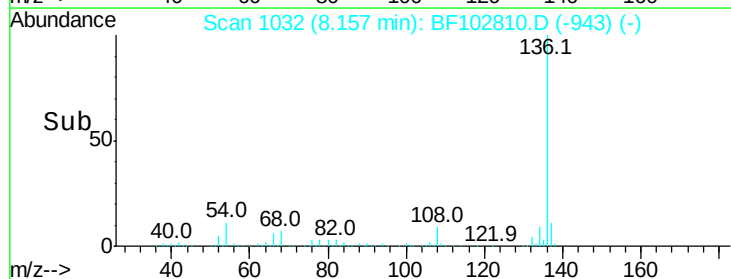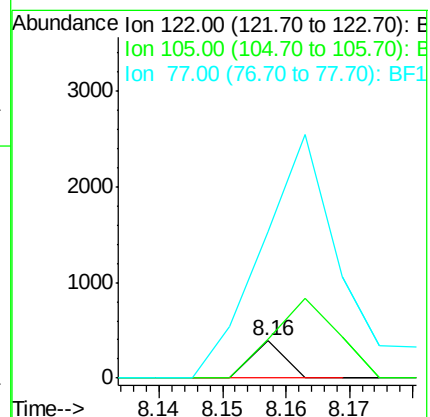







#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.92 min Scan# 1331
Delta R.T. -0.01 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
164	100		
162	102.7	86.1	129.1
160	44.9	38.3	57.5

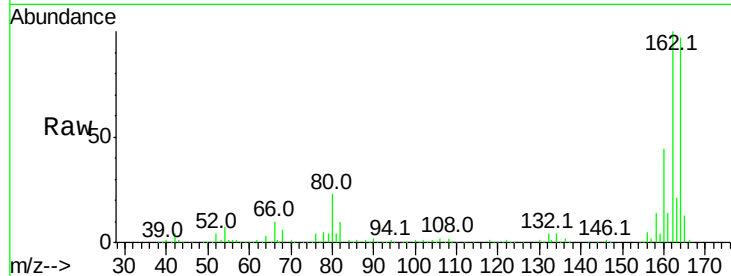


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


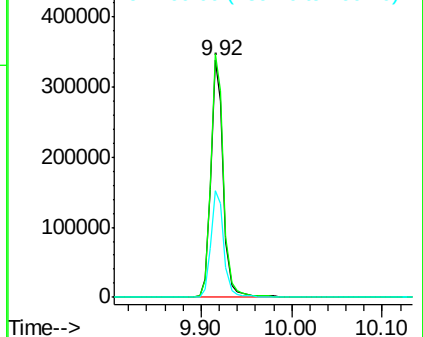



#41
2,4,6-Tribromophenol
Concen: 61.946 ng
RT: 10.70 min Scan# 1465
Delta R.T. -0.01 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Tgt Ion	Ratio	Lower	Upper
330	100		
332	105.8	77.0	115.6
141	40.4	29.9	44.9

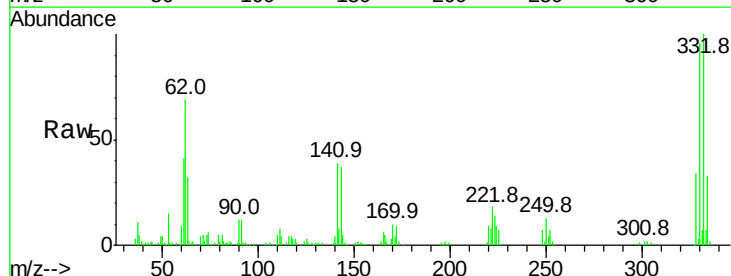

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




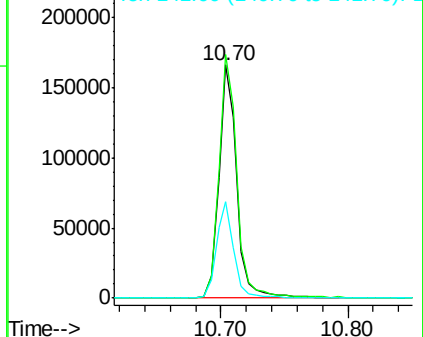


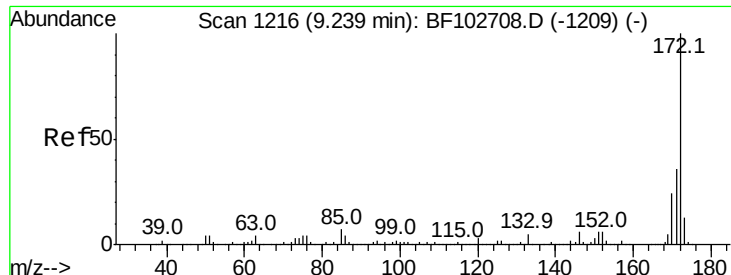

#44
2-Fluorobiphenyl
Concen: 46.553 ng
RT: 9.23 min Scan# 1215
Delta R.T. -0.01 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53




Instrument :
BNA_F
ClientSampleId :


Tot Ion:172 Resp: 925970
Ion Ratio Lower Upper
172 100
171 35.8 29.7 44.5
170 24.6 19.6 29.4

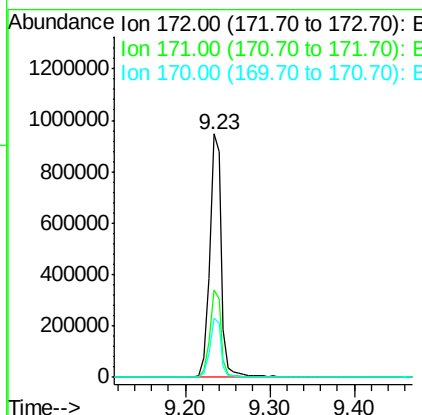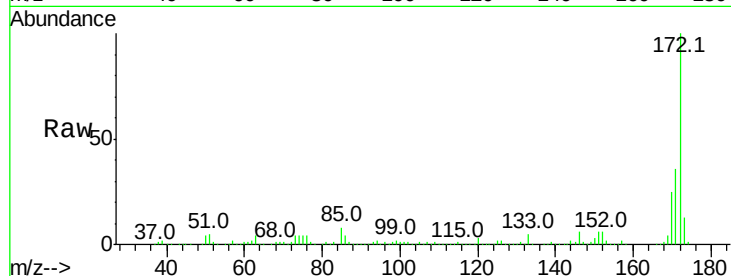

#47
2-Nitroaniline
Concen: 3.592 ng
RT: 9.63 min Scan# 1282
Delta R.T. 0.16 min
Lab File: BF102810.D
Acq: 7 Feb 2018 12:53

Tgt Ion: 65 Resp: 874
Ion Ratio Lower Upper
65 100
92 545.8 55.8 83.6#
138 0.0 91.2 136.8#

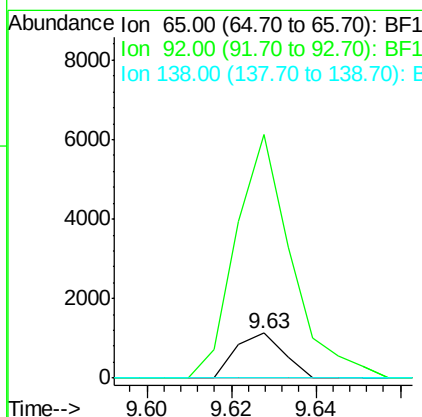

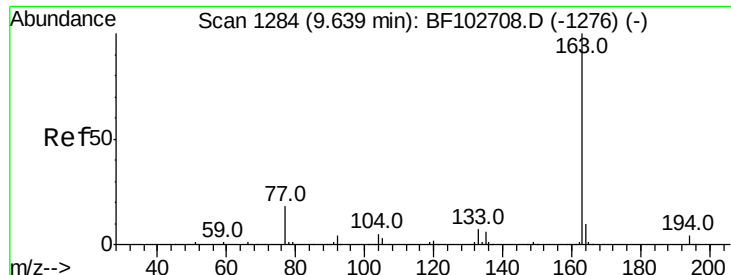

#49

Dimethylphthalate

Concen: 2.688 ng

RT: 9.63 min Scan# 1282

Delta R.T. -0.02 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 69167

Ion Ratio Lower Upper

163 100

194 3.1 2.7 4.1




164 10.2 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

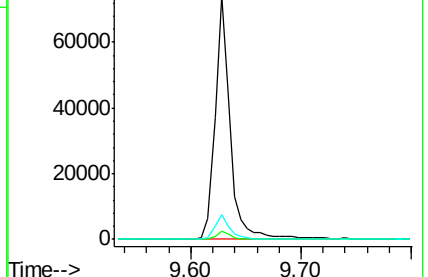

#50

2,6-Dinitrotoluene

Concen: 8.642 ng

RT: 9.92 min Scan# 1331

Delta R.T. 0.21 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53


Tgt Ion:165 Resp: 42313

Ion Ratio Lower Upper

165 100

63 1.3 44.7 67.1#



89 1.1 44.0 66.0#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1




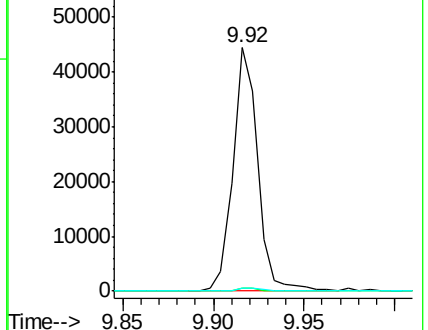




#56
 2,4-Dinitrotoluene
 Concen: 9.106 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.19 min
 Lab File: BF102810.D
 Acq: 7 Feb 2018 12:53




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:165 Resp: 42313
 Ion Ratio Lower Upper
 165 100
 63 1.3 36.4 54.6#
 89 1.1 57.8 86.6#
 182 0.0 1.6 2.4#

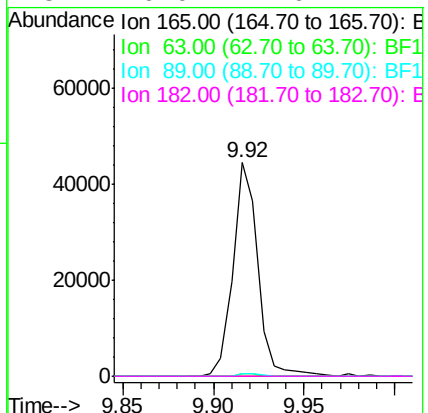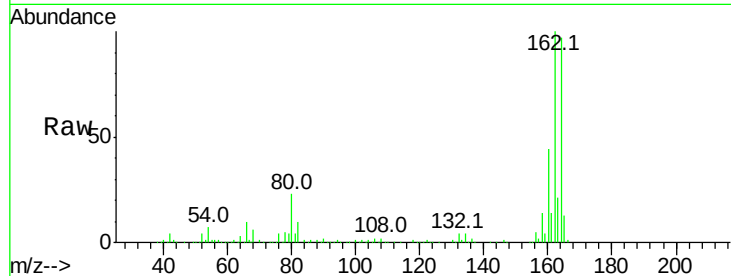

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.40 min Scan# 1584
 Delta R.T. -0.01 min
 Lab File: BF102810.D
 Acq: 7 Feb 2018 12:53

Tgt Ion:188 Resp: 586439
 Ion Ratio Lower Upper
 188 100
 94 11.4 8.5 12.7
 80 12.7 9.2 13.8

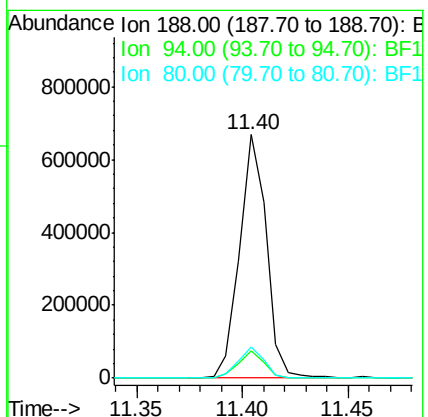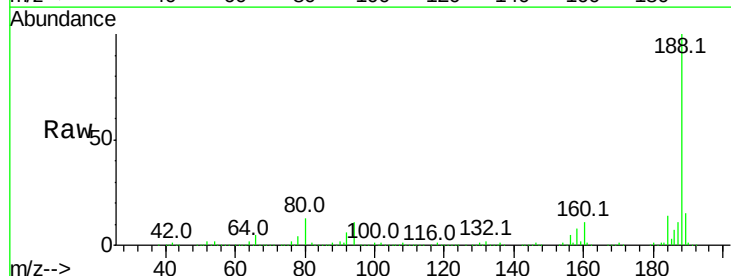


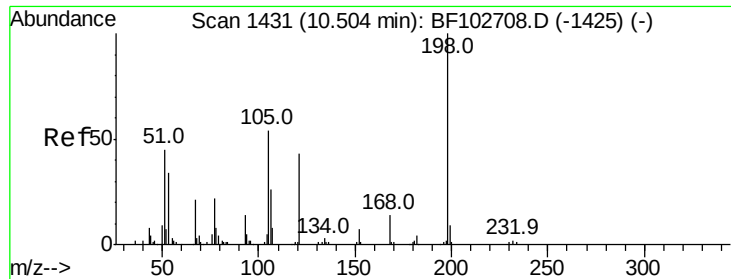




#64
 4,6-Dinitro-2-methylphenol
 Concen: 8.944 ng
 RT: 10.70 min Scan# 1464
 Delta R.T. 0.18 min
 Lab File: BF102810.D
 Acq: 7 Feb 2018 12:53

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:198 Resp: 401
 Ion Ratio Lower Upper
 198 100
 51 220.6 37.7 77.7#
 105 158.2 36.3 76.3#

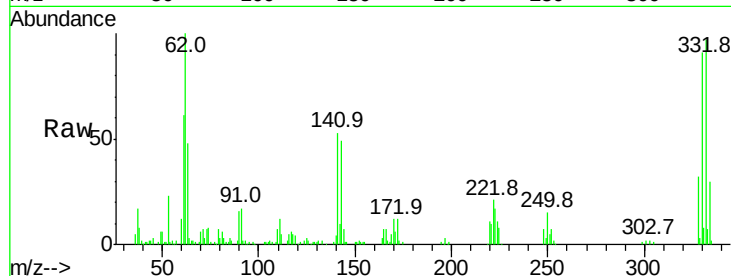


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E


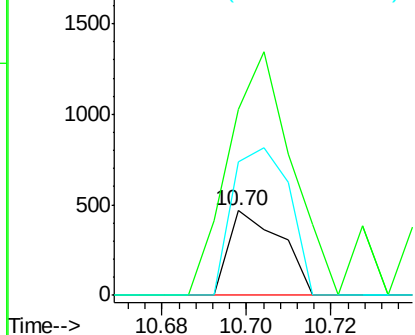



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.04 min Scan# 2033
 Delta R.T. -0.01 min
 Lab File: BF102810.D
 Acq: 7 Feb 2018 12:53

Tgt Ion:240 Resp: 449887
 Ion Ratio Lower Upper
 240 100
 120 13.4 9.5 14.3
 236 27.1 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

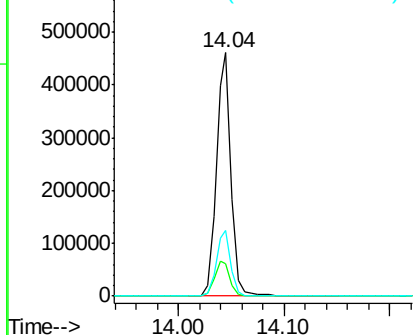

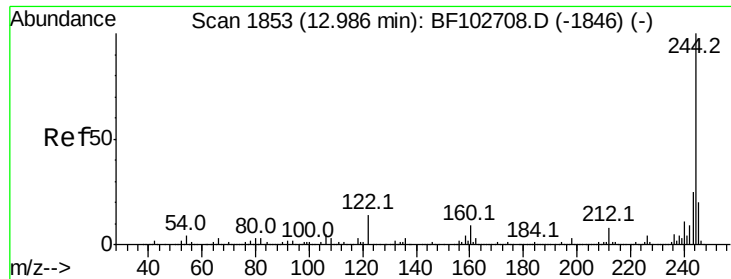

#78

Terphenyl-d14

Concen: 47.179 ng

RT: 12.99 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 896417

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0




122 16.0 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

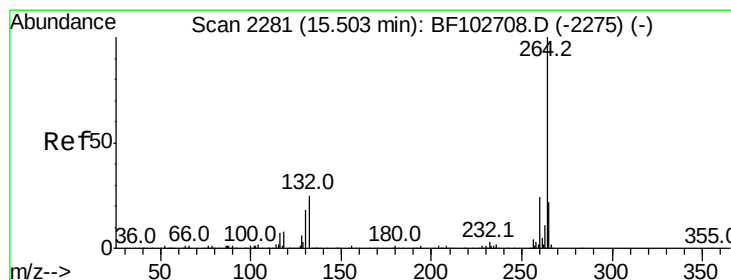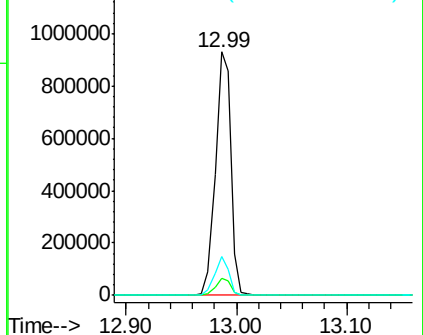

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.52 min Scan# 2284

Delta R.T. -0.01 min

Lab File: BF102810.D

Acq: 7 Feb 2018 12:53


Tgt Ion:264 Resp: 350316

Ion Ratio Lower Upper

264 100

260 25.3 19.2 28.8

265 21.3 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

