
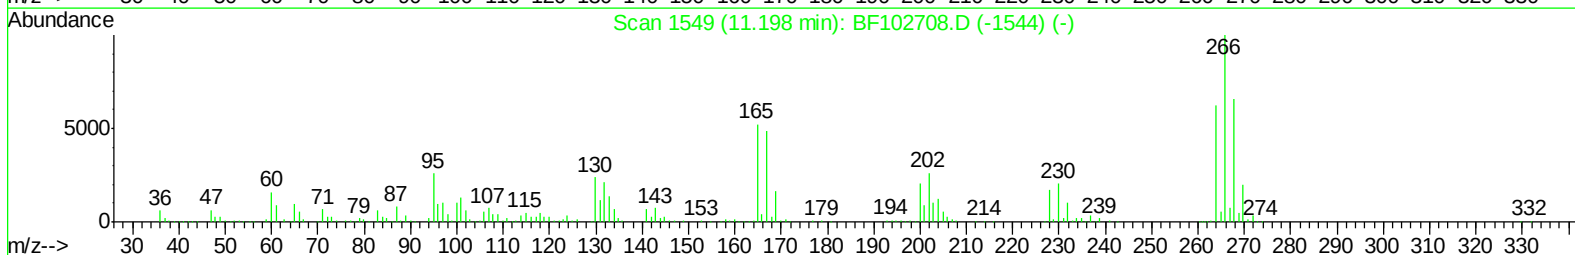
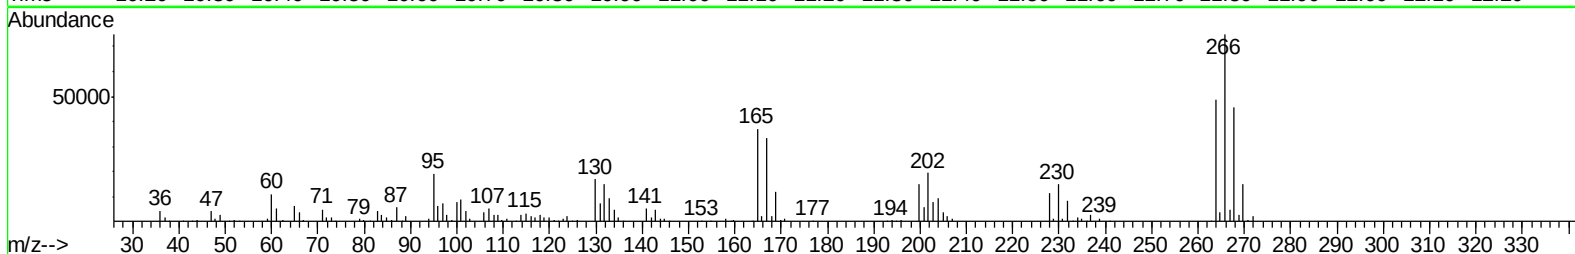


Data Path : Z:\HPCHEM1\BNA F\DATA\BF020718\
Data File : BF102817.D
Acq On : 7 Feb 2018 16:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 07:30:56 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

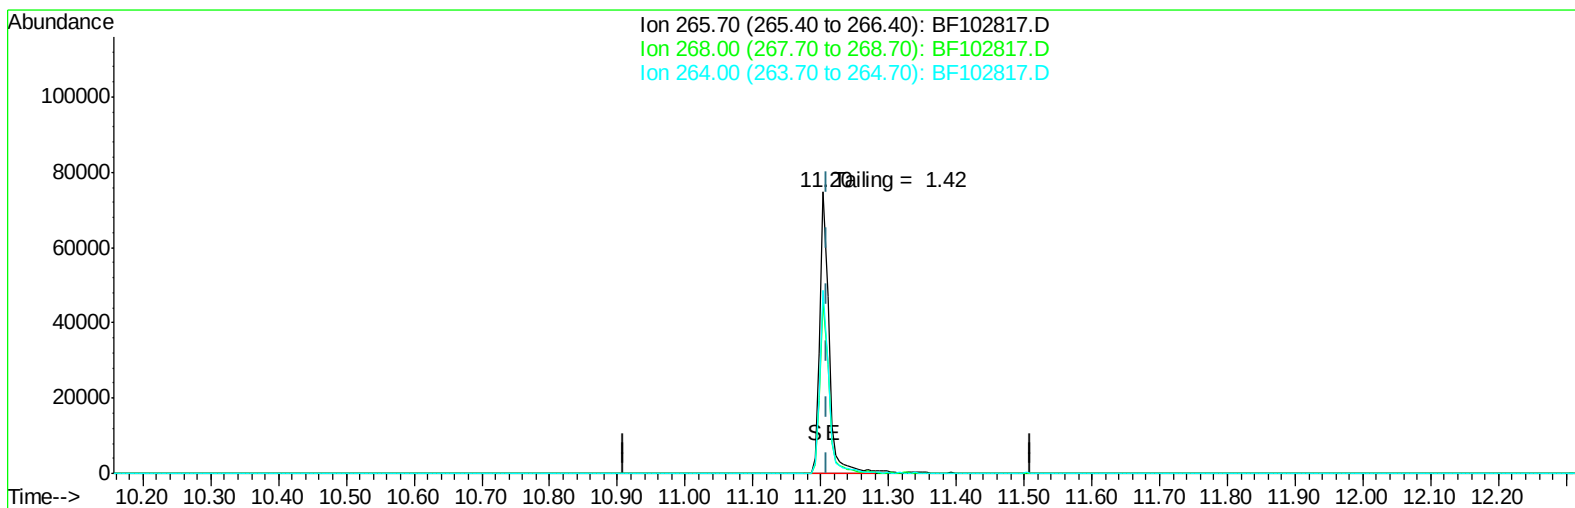

TIC: BF102817.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 30904.86ng

response 68170

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.13
264.00	61.90	64.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020718\
Data File : BF102817.D
Acq On : 7 Feb 2018 16:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 07:30:56 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

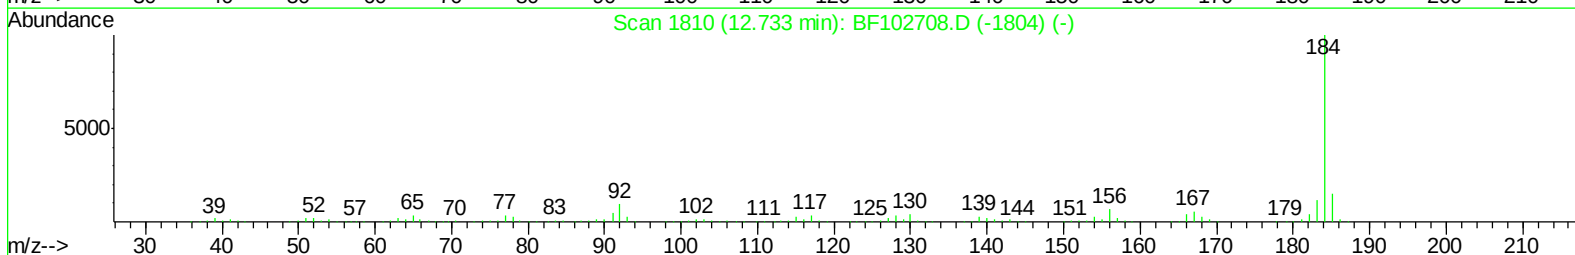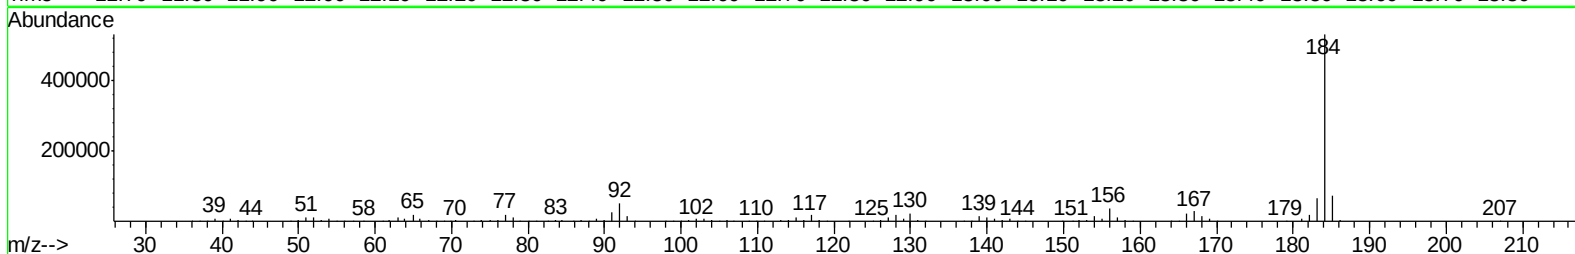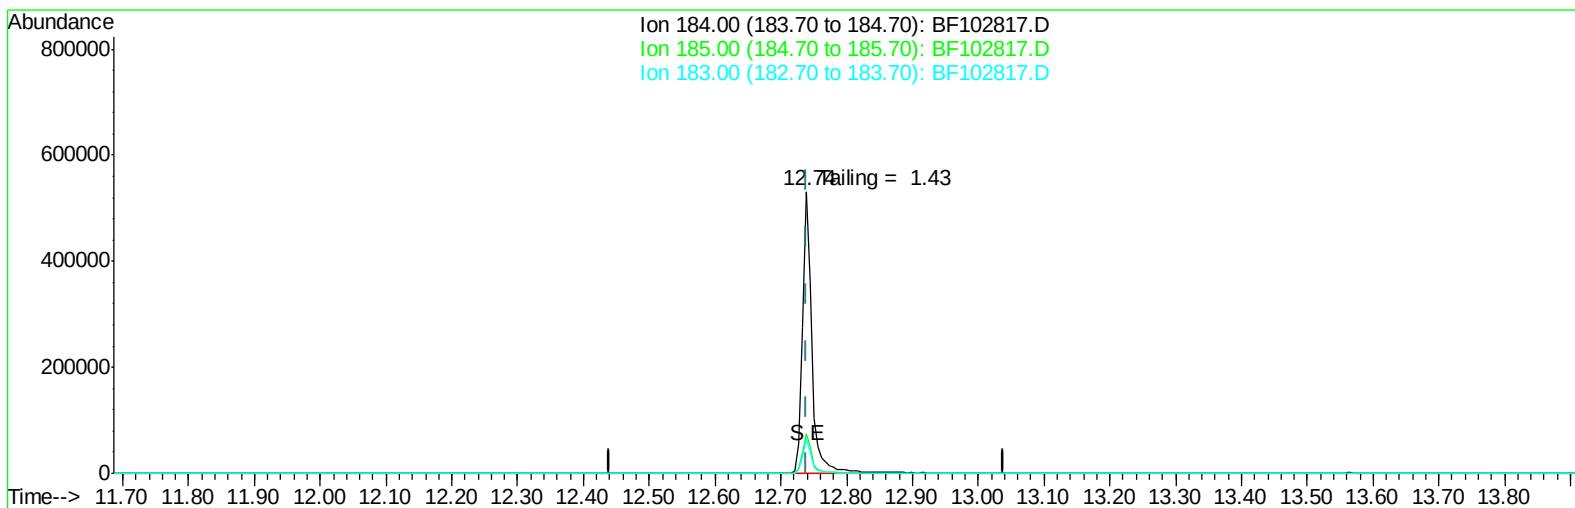

TIC: BF102817.D

(76) Benzidine

12.739min (+0.000) 0.00ng

response 538184

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.04
183.00	11.60	12.25
0.00	0.00	0.00