


Data Path : Z:\HPCHEM1\BNA F\Data\BF020718\
 Data File : BF102805.D
 Acq On : 7 Feb 2018 10:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

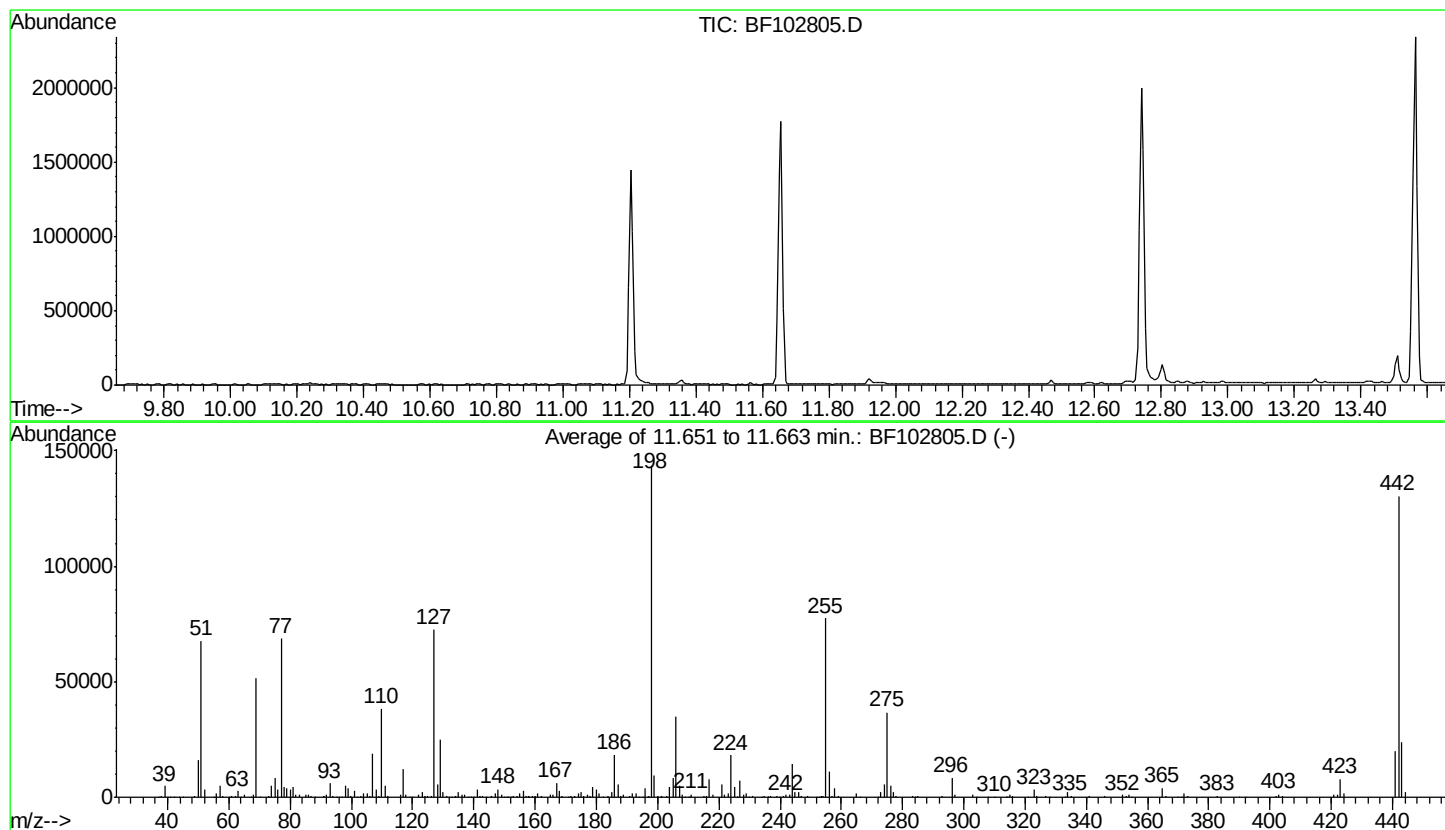

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	67622	PASS
68	69	0.00	2	1.7	861	PASS
69	198	0.00	100	35.9	51573	PASS
70	69	0.00	2	0.5	265	PASS
127	198	10	80	50.5	72512	PASS
197	198	0.00	2	0.5	731	PASS
198	198	100	100	100.0	143549	PASS
199	198	5	9	6.6	9431	PASS
275	198	10	60	25.7	36842	PASS
365	198	1	100	2.9	4110	PASS
441	443	0.01	100	84.2	19954	PASS
442	198	50	100	90.8	130373	PASS
443	442	15	24	18.2	23696	PASS