


Data Path : Z:\HPCHEM1\BNA F\Data\BF020718\
 Data File : BF102817.D
 Acq On : 7 Feb 2018 16:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

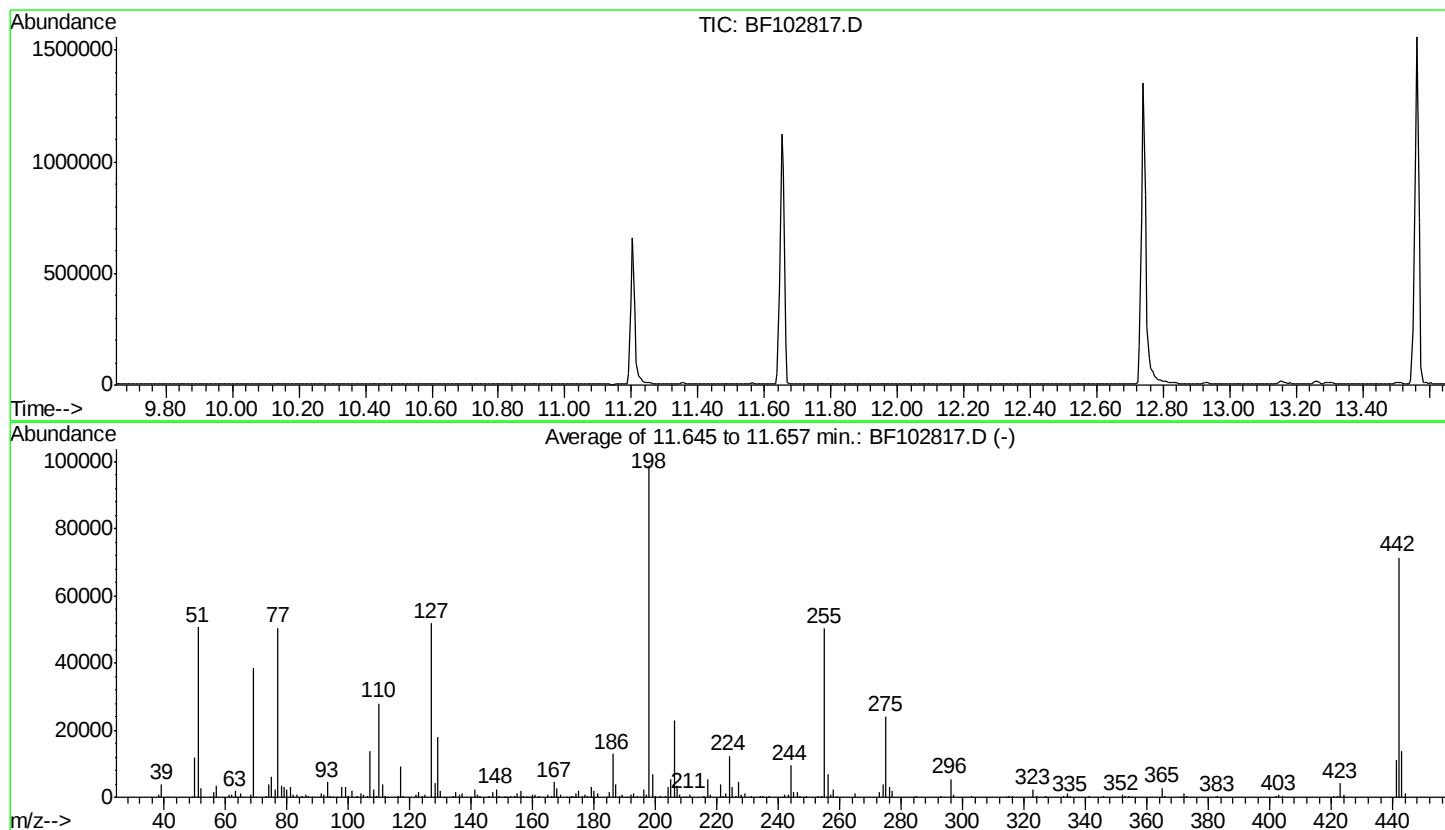

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	50681	PASS
68	69	0.00	2	1.8	691	PASS
69	198	0.00	100	39.0	38602	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	52.4	51762	PASS
197	198	0.00	2	0.6	610	PASS
198	198	100	100	100.0	98866	PASS
199	198	5	9	6.8	6696	PASS
275	198	10	60	24.3	23982	PASS
365	198	1	100	2.8	2749	PASS
441	443	0.01	100	80.2	11048	PASS
442	198	50	100	72.2	71414	PASS
443	442	15	24	19.3	13783	PASS