
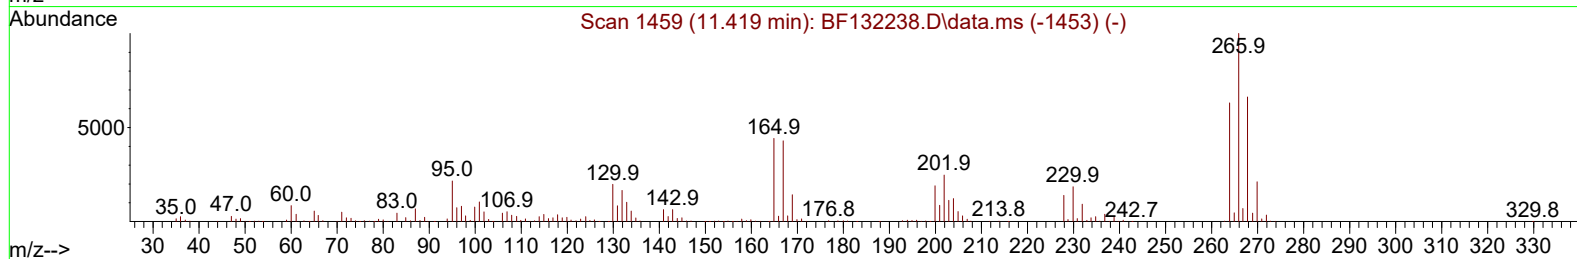
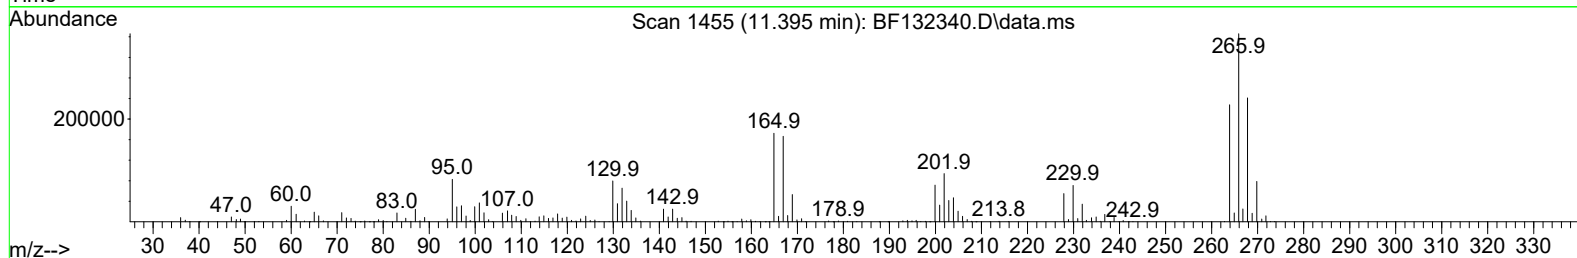


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020723\
Data File : BF132340.D
Acq On : 07 Feb 2023 12:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:06:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:05:36 2023
Response via : Initial Calibration

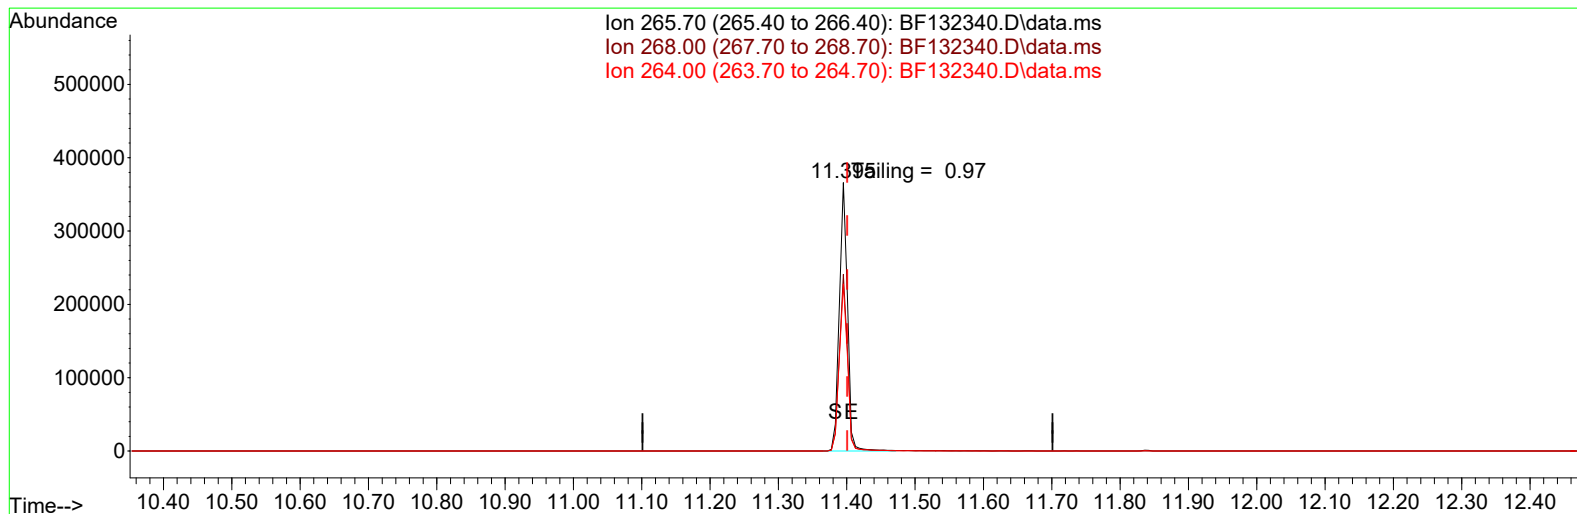

TIC: BF132340.D\data.ms

(70) Pentachlorophenol (C)




11.395min (-0.006) 520815.32 ng

response 305493

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.85
264.00	63.10	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020723\
 Data File : BF132340.D
 Acq On : 07 Feb 2023 12:06
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:06:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 07 04:05:36 2023
 Response via : Initial Calibration

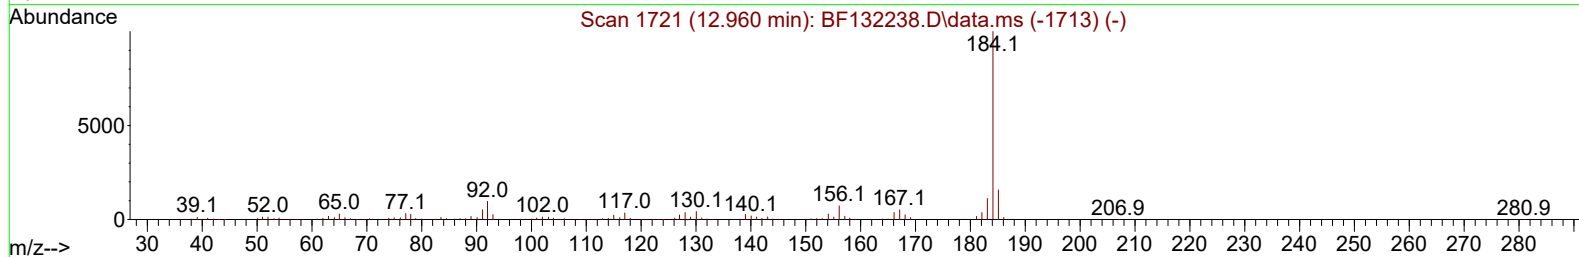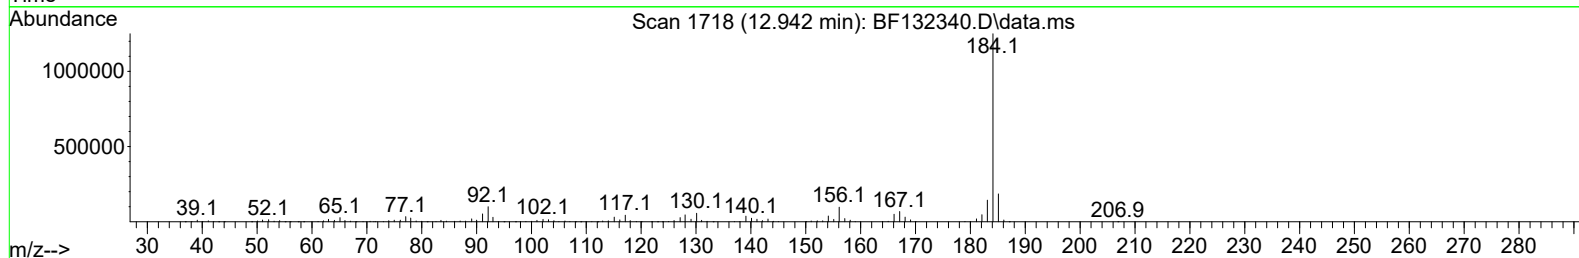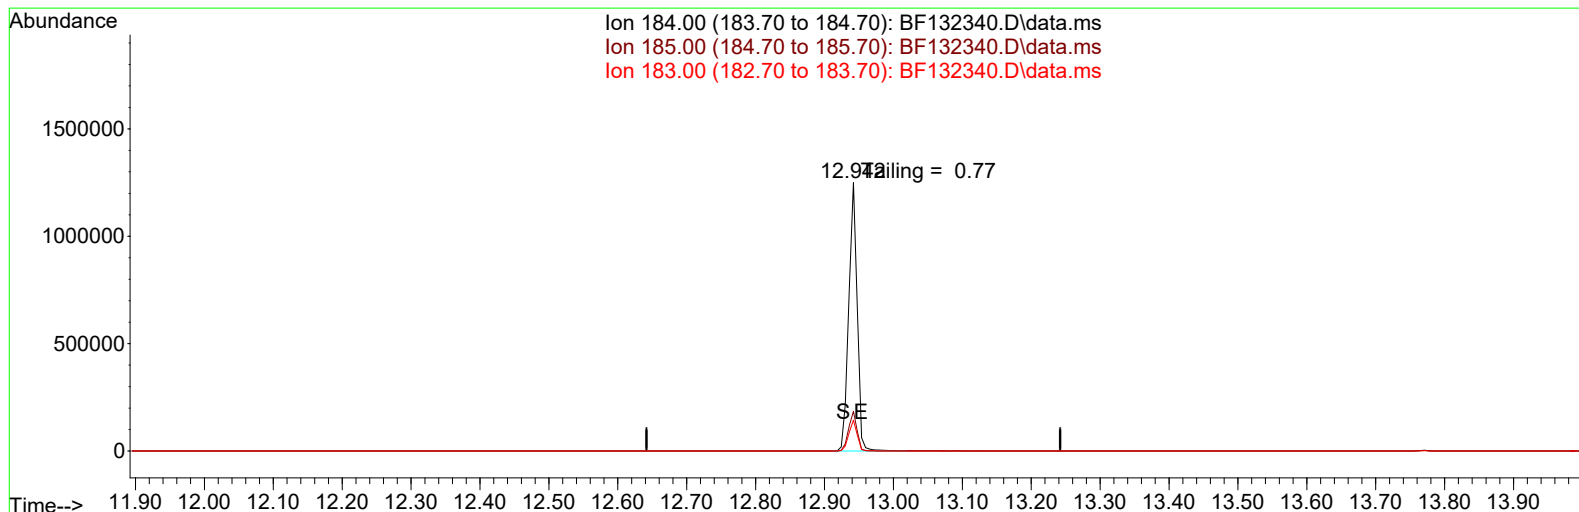

TIC: BF132340.D\data.ms

(77) Benzidine

12.942min (-12.942) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.70	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00