
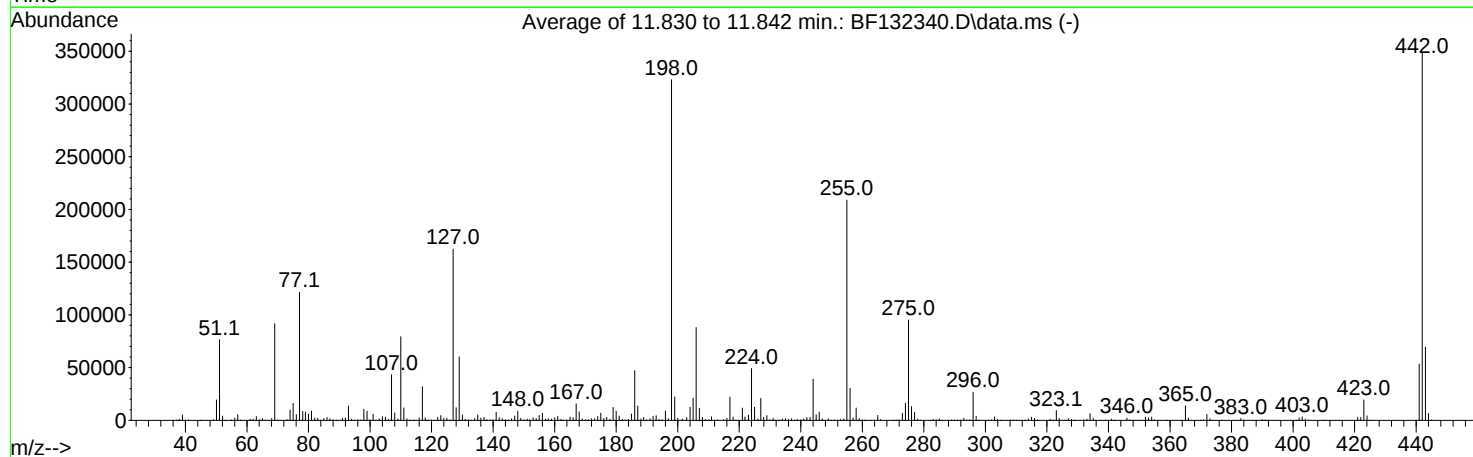


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020723\
 Data File : BF132340.D
 Acq On : 07 Feb 2023 12:06
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 07 04:05:36 2023

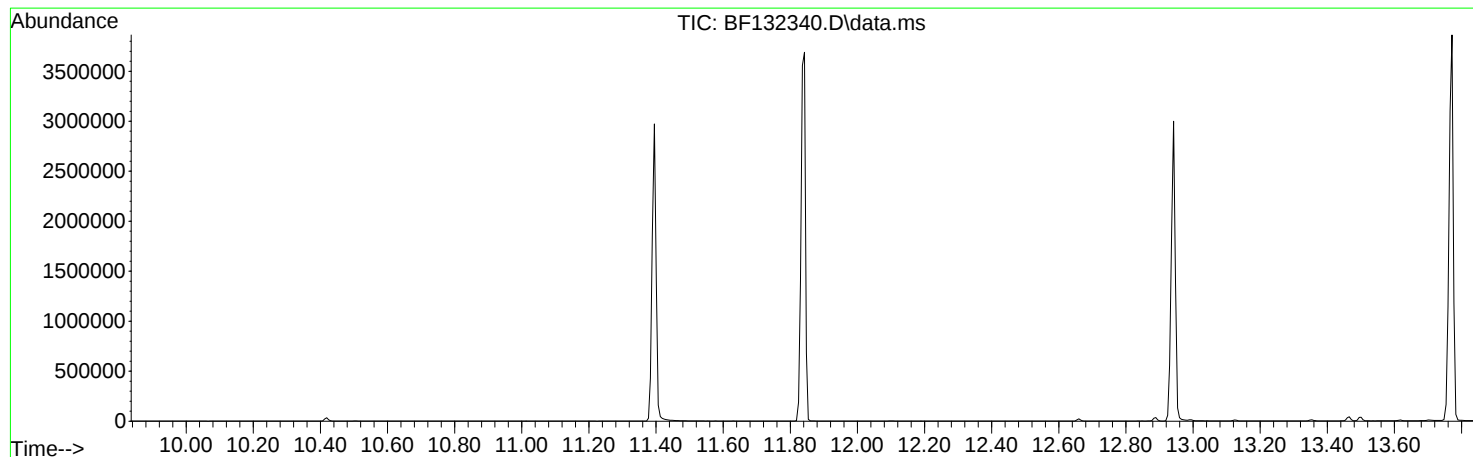




AutoFind: Scans 1529, 1530, 1531; Background Corrected with Scan 1524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	76363	PASS
68	69	0.00	2	1.7	1574	PASS
69	198	0.00	100	28.4	91629	PASS
70	69	0.00	2	0.5	438	PASS
127	198	10	80	50.2	162240	PASS
197	198	0.00	2	0.5	1517	PASS
198	198	100	100	100.0	323093	PASS
199	198	5	9	6.9	22186	PASS
275	198	10	60	29.4	95059	PASS
365	198	1	100	4.3	13756	PASS
441	198	0.01	100	16.5	53293	PASS
442	442	50	100	100.0	348920	PASS
443	442	15	24	19.8	69221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020723\
Data File : BF132340.D
Acq On : 07 Feb 2023 12:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:06:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:05:36 2023
Response via : Initial Calibration

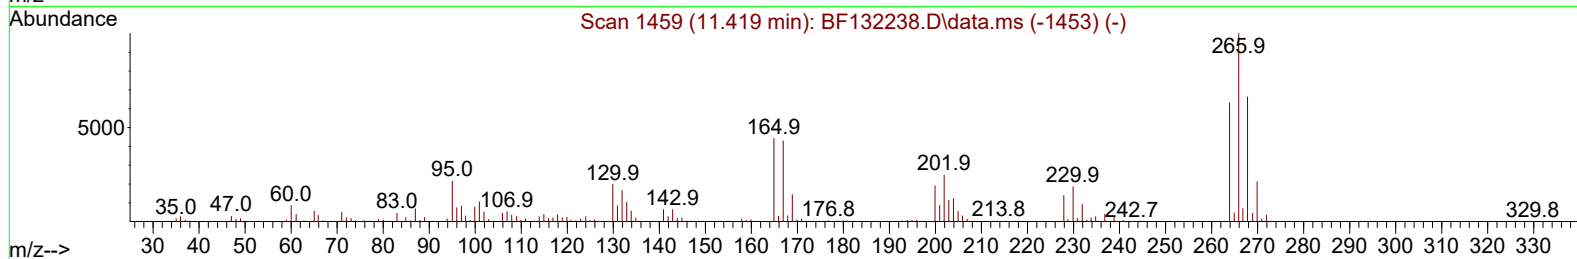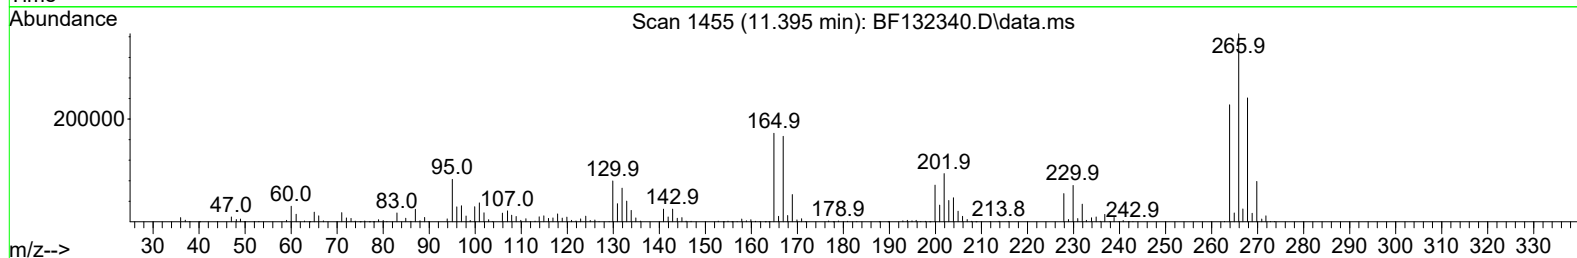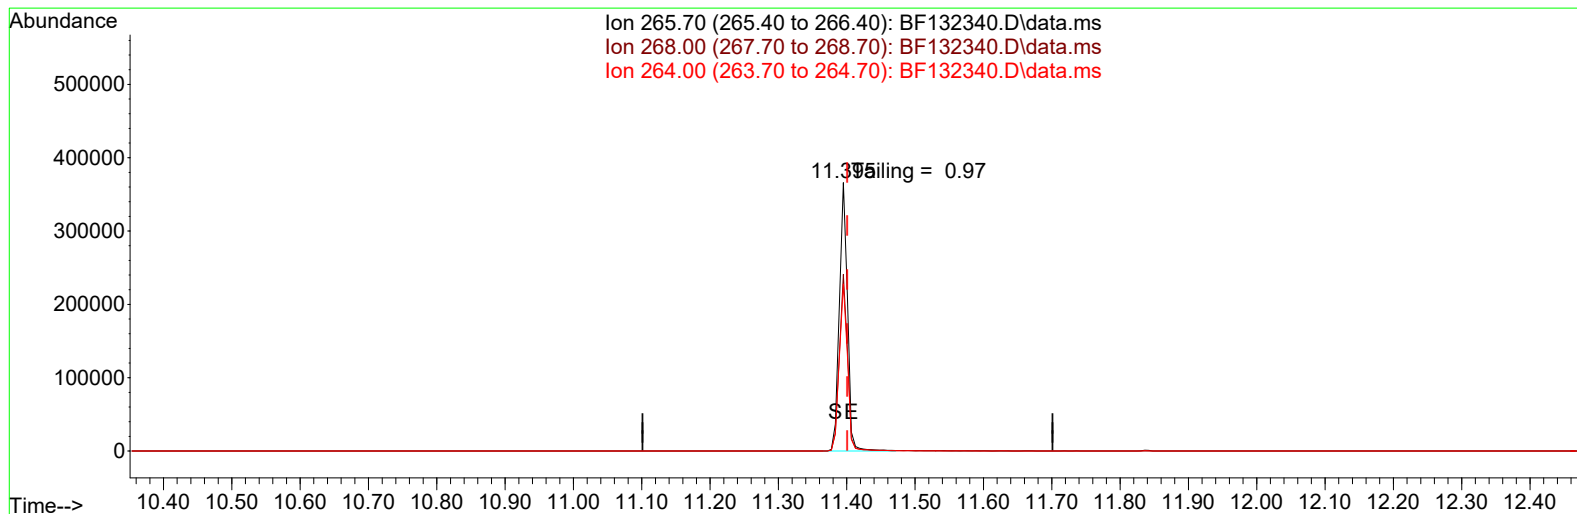

TIC: BF132340.D\data.ms

(70) Pentachlorophenol (C)

11.395min (-0.006) 520815.32 ng




response 305493

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.85
264.00	63.10	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020723\
Data File : BF132340.D
Acq On : 07 Feb 2023 12:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:06:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:05:36 2023
Response via : Initial Calibration

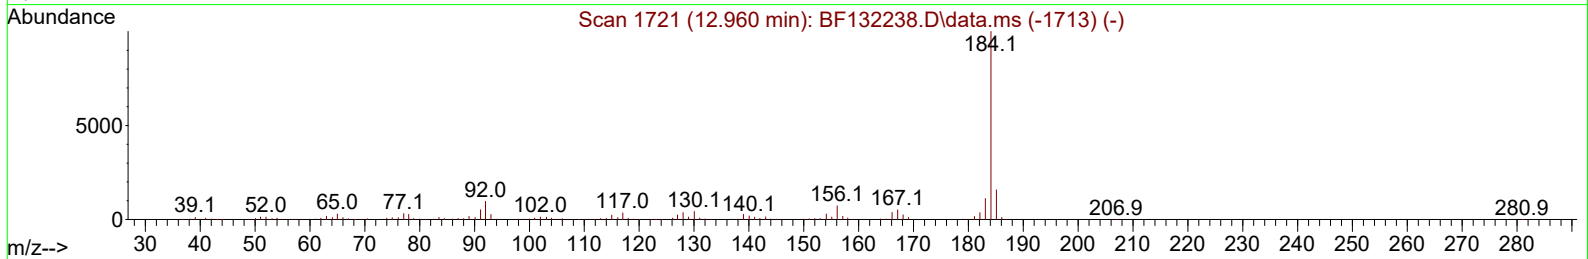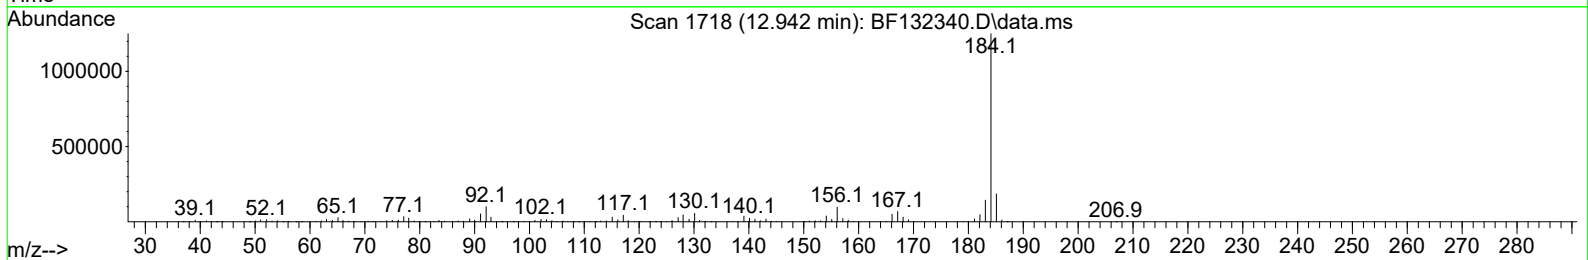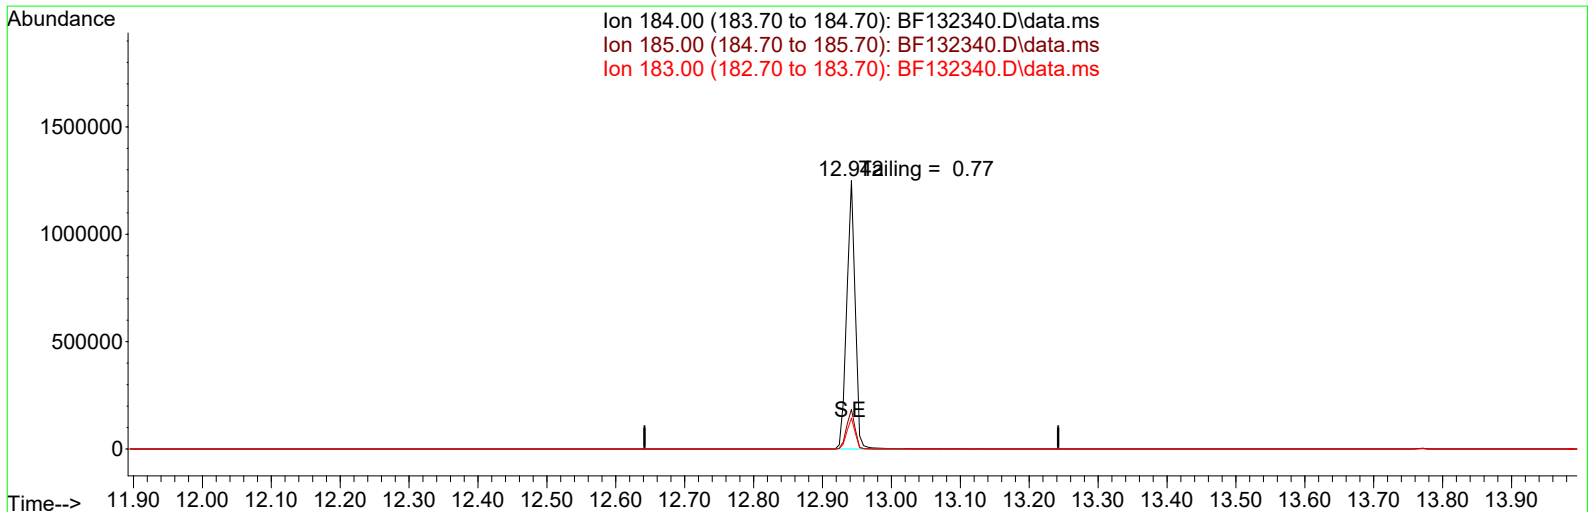

TIC: BF132340.D\data.ms

(77) Benzidine

12.942min (-12.942) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.70	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2023	BNA_F	<u>BF132340.D</u>
Compound Name	Response	Retention Time
DDT	672964	13.771
DDD	13708	13.465
DDE	1843	13.124
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15551	688515	2.26

Instrument :
BNA_F
ClientSampleId :
DFTPP