


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020724\
Data File : BF137311.D
Acq On : 07 Feb 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 31 04:56:22 2024

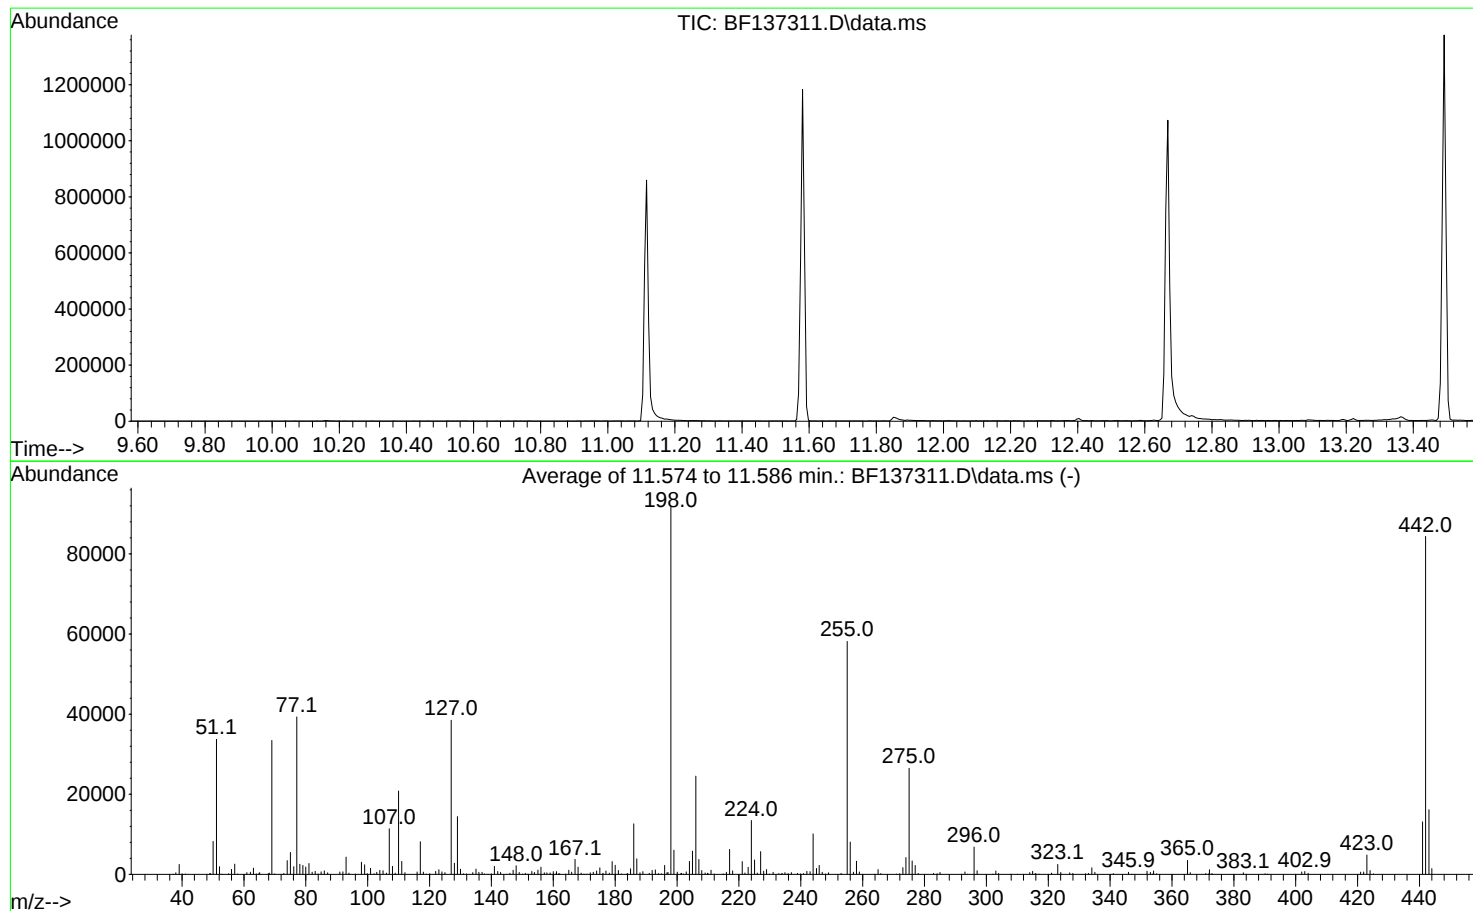




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	33727	PASS
68	69	0.00	2	0.9	315	PASS
69	198	0.00	100	36.4	33422	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	41.9	38483	PASS
197	198	0.00	2	0.5	474	PASS
198	198	100	100	100.0	91840	PASS
199	198	5	9	6.6	6027	PASS
275	198	10	60	28.8	26495	PASS
365	198	1	100	3.8	3483	PASS
441	198	0.01	100	14.3	13121	PASS
442	442	50	100	100.0	84355	PASS
443	442	15	24	19.1	16142	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020724\
Data File : BF137311.D
Acq On : 07 Feb 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 11:56:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

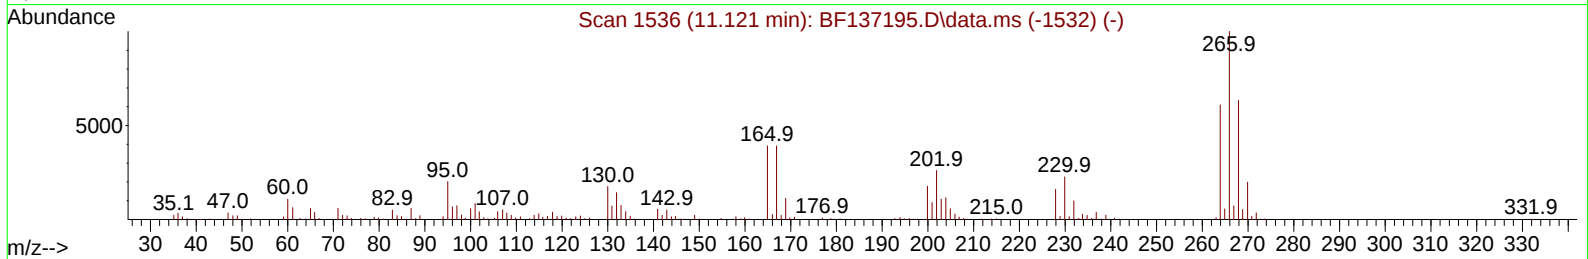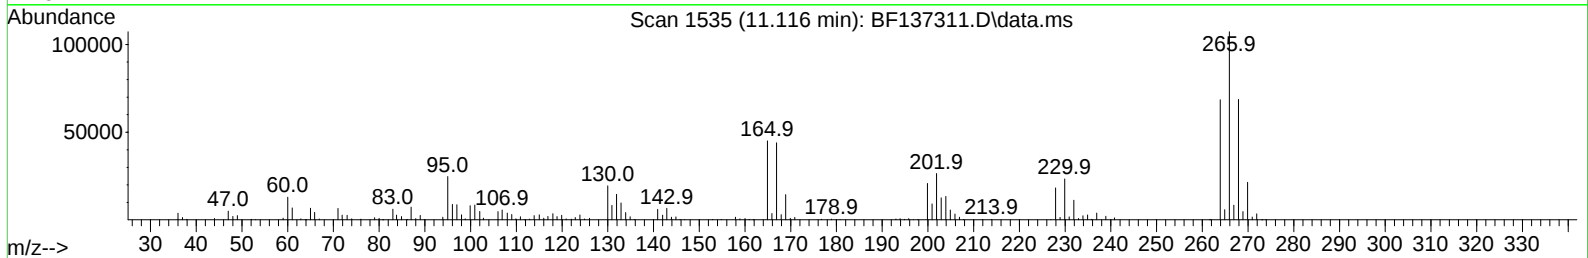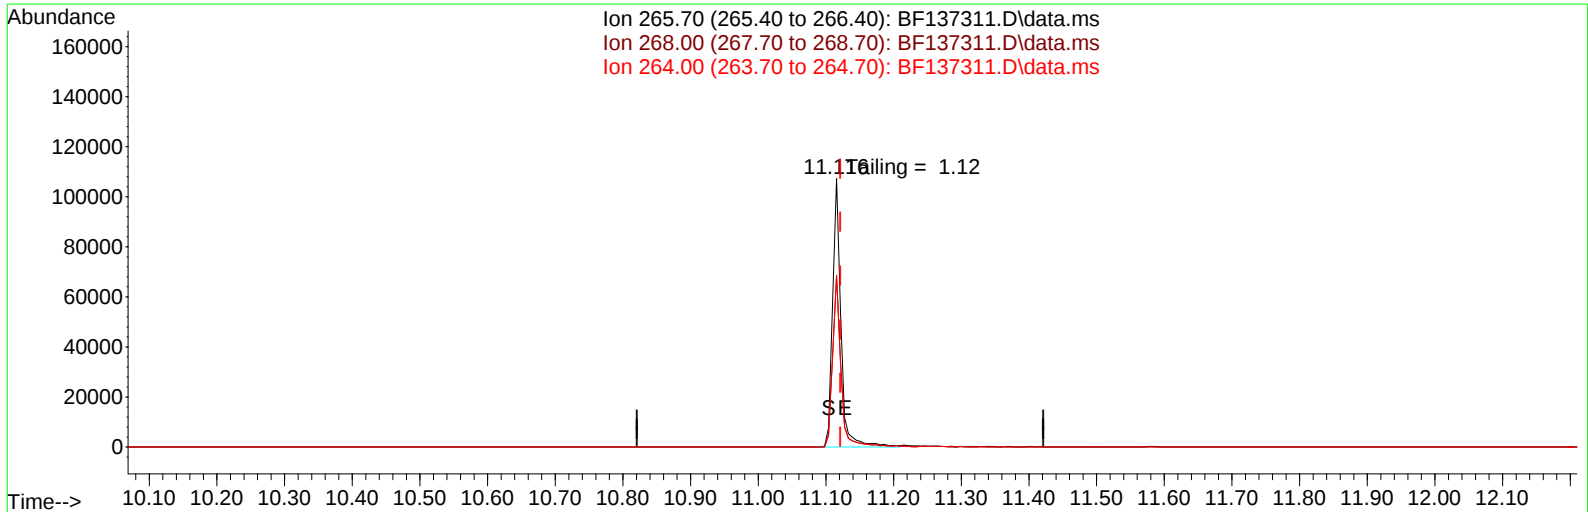

TIC: BF137311.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.005) 29995.58 ng

response 92500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.06
264.00	61.00	63.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2024	BNA_F	<u>BF137311.D</u>
Compound Name	Response	Retention Time
DDT	213687	13.492
DDD	2992	13.221
DDE	202	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3194	216881	1.47

Instrument :
BNA_F
ClientSampleId :
DFTPP