
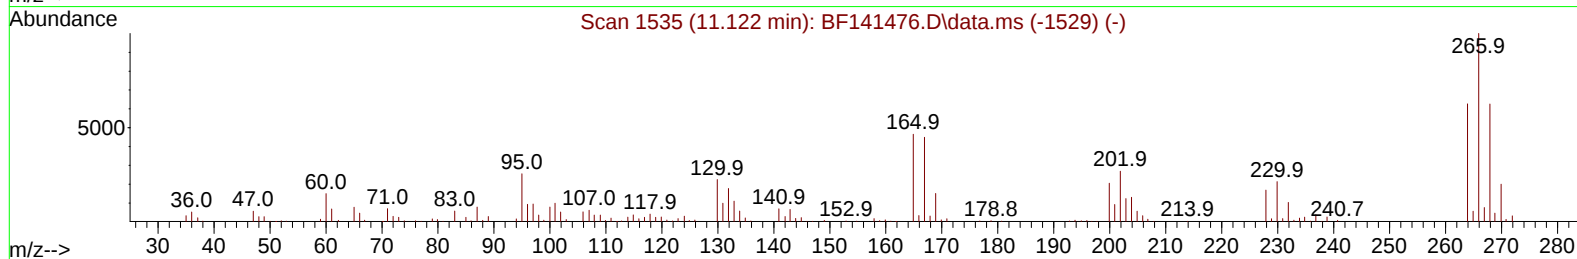
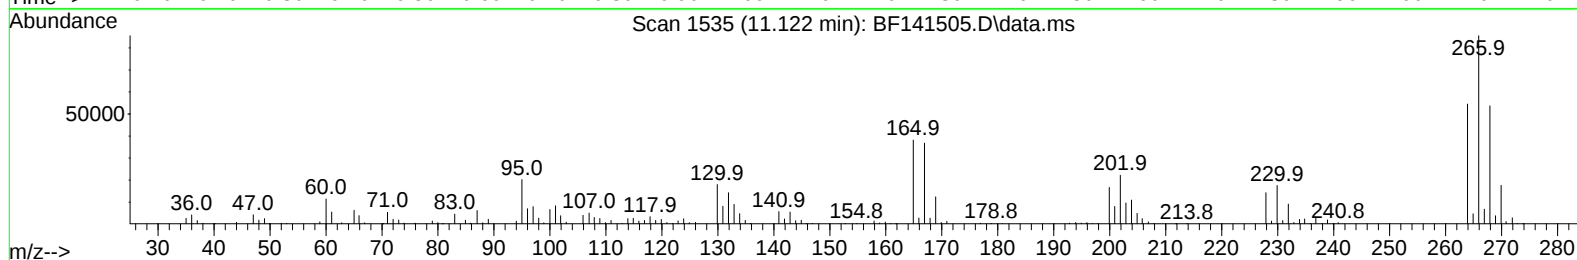


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141505.D
Acq On : 07 Feb 2025 14:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 14:31:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

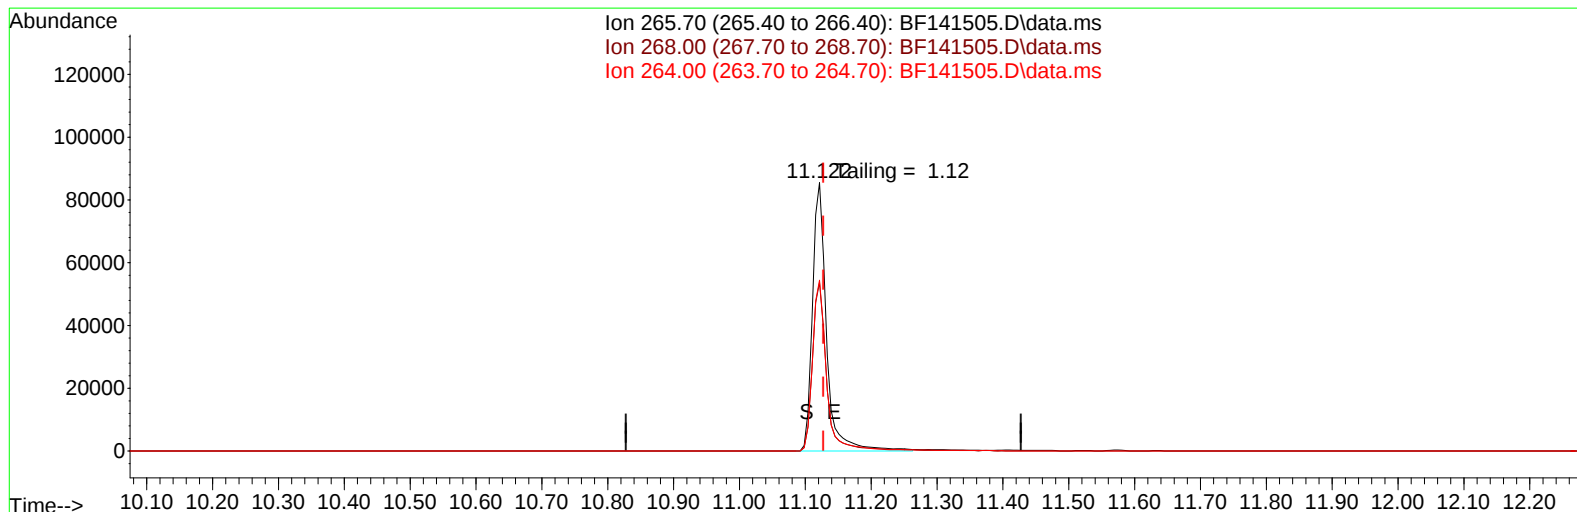

TIC: BF141505.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.006) 20208.15 ng

response 127294

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.80
264.00	62.60	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141505.D
Acq On : 07 Feb 2025 14:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 14:31:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

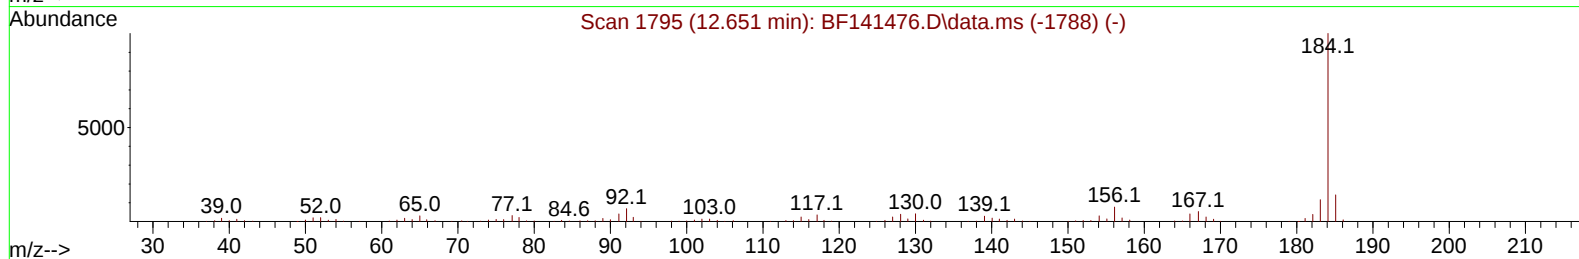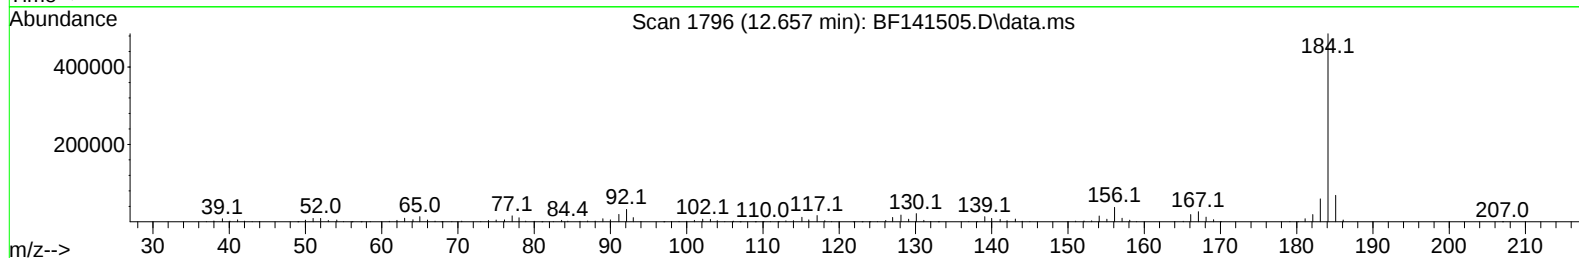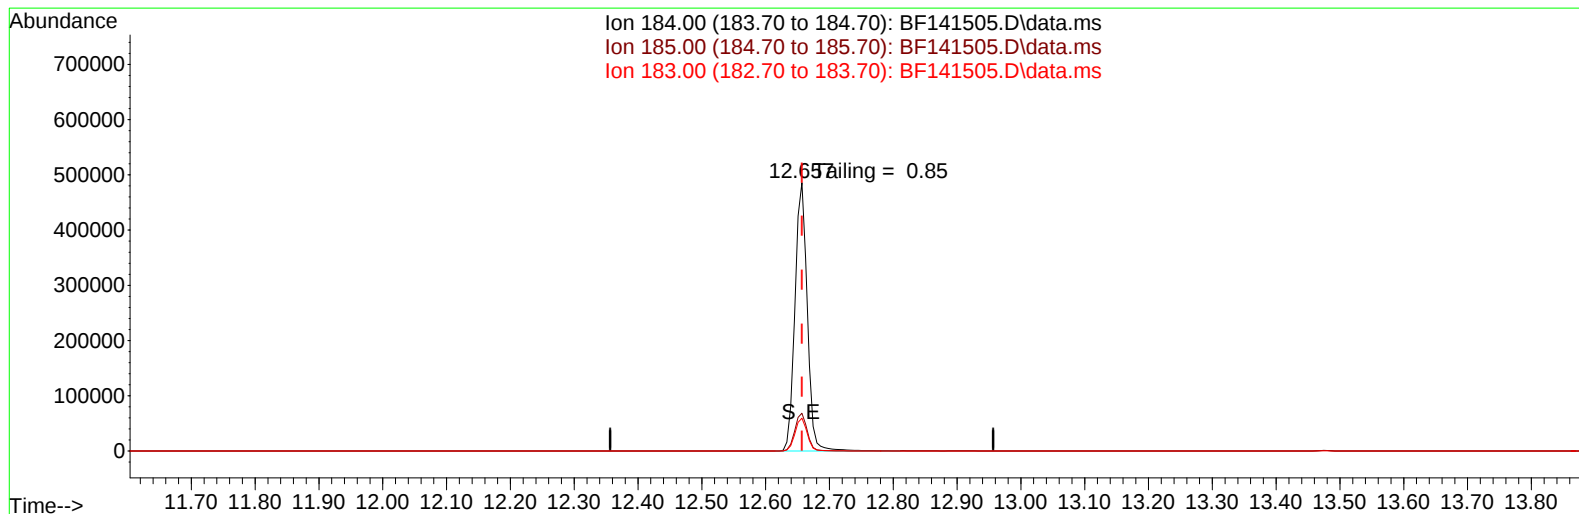

TIC: BF141505.D\data.ms

(77) Benzidine

12.657min (+ 0.000) 44608.91 ng

response 656208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.60	12.23
0.00	0.00	0.00