

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
 Data File : BF141503.D
 Acq On : 07 Feb 2025 12:58
 Operator : RC/JU
 Sample : PB166580BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166580BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	559	565	587	rBV	2019978	2680574	73.09%	13.141%
2	6.428	730	737	766	rBV	1902018	2719647	74.15%	13.332%
3	6.786	793	798	809	rVB	416383	511587	13.95%	2.508%
4	7.351	887	894	899	rBV	1284658	1790933	48.83%	8.779%
5	8.069	1010	1016	1037	rBV	503281	675433	18.42%	3.311%
6	9.145	1192	1199	1225	rBV	2506305	3351436	91.38%	16.429%
7	9.822	1308	1314	1330	rVB	601183	787796	21.48%	3.862%
8	10.616	1443	1449	1470	rBV	1563707	2099399	57.24%	10.292%
9	11.310	1562	1567	1576	rBV	638832	828047	22.58%	4.059%
10	12.904	1831	1838	1843	rBV	2706335	3667600	100.00%	17.979%
11	13.951	2011	2016	2032	rBV	548568	723638	19.73%	3.547%
12	15.404	2257	2263	2279	rBV	341241	562976	15.35%	2.760%




Sum of corrected areas: 20399066

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141503.D
Acq On : 07 Feb 2025 12:58
Operator : RC/JU
Sample : PB166580BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166580BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

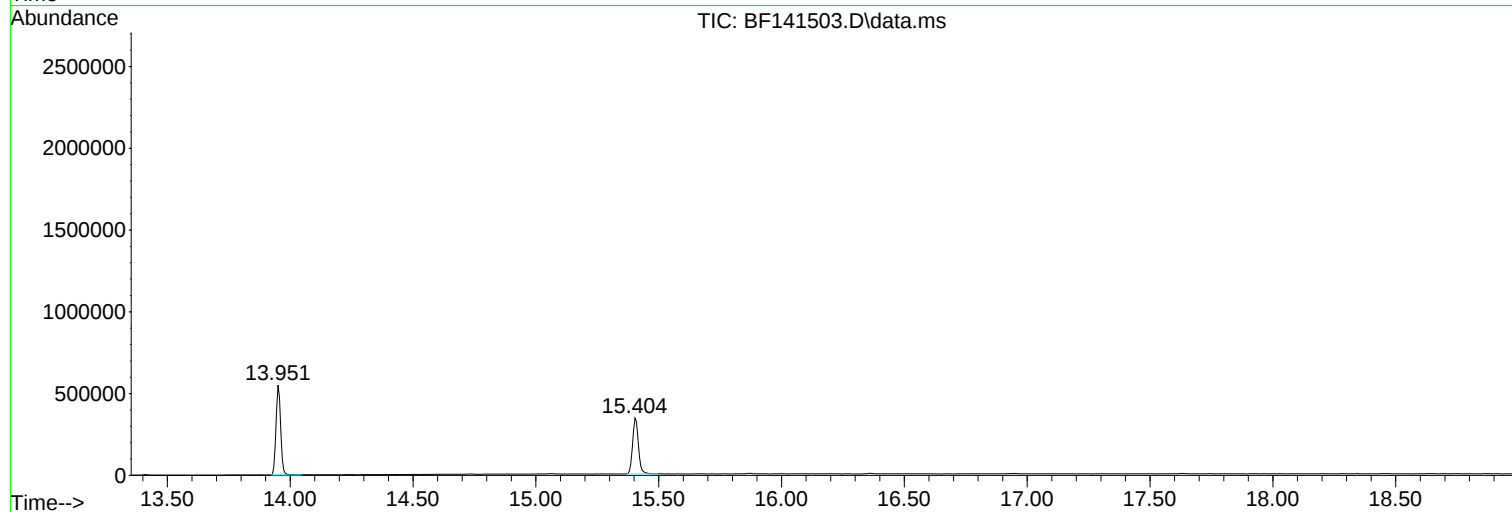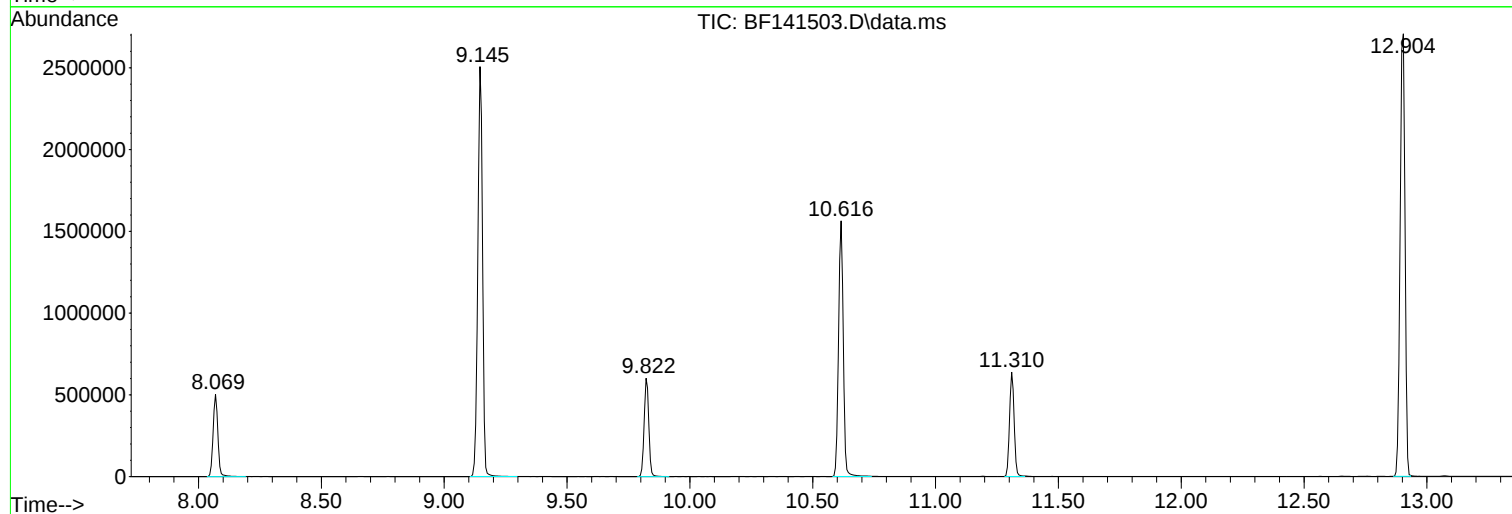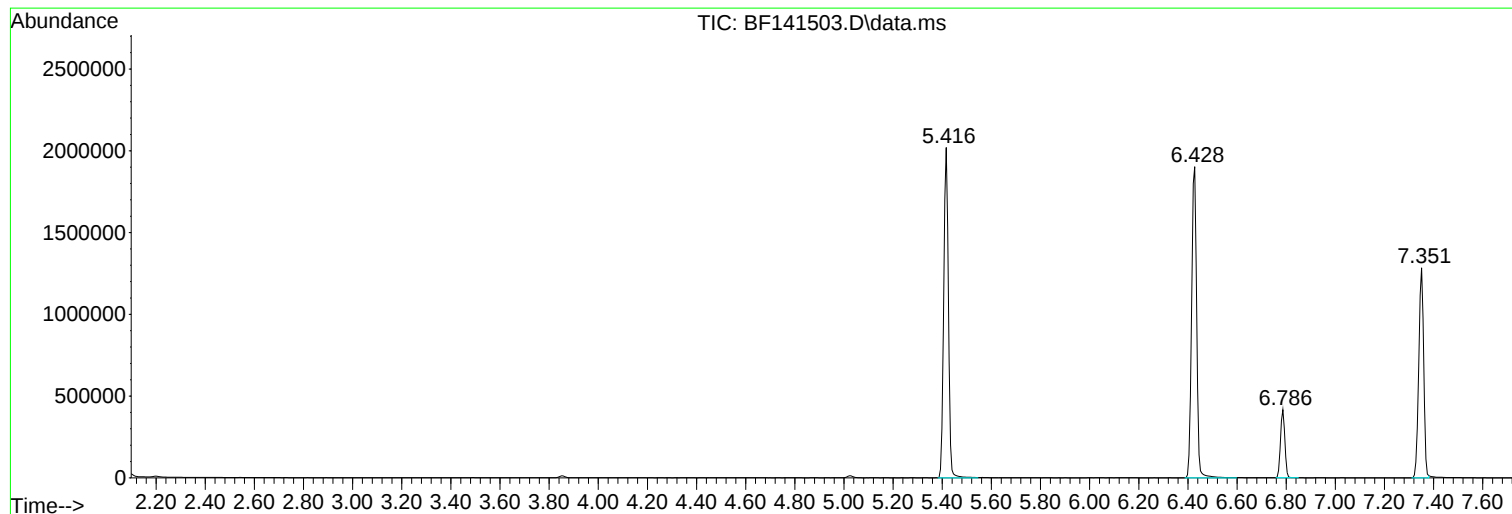

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141503.D
Acq On : 07 Feb 2025 12:58
Operator : RC/JU
Sample : PB166580BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166580BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141503.D
Acq On : 07 Feb 2025 12:58
Operator : RC/JU
Sample : PB166580BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166580BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------