
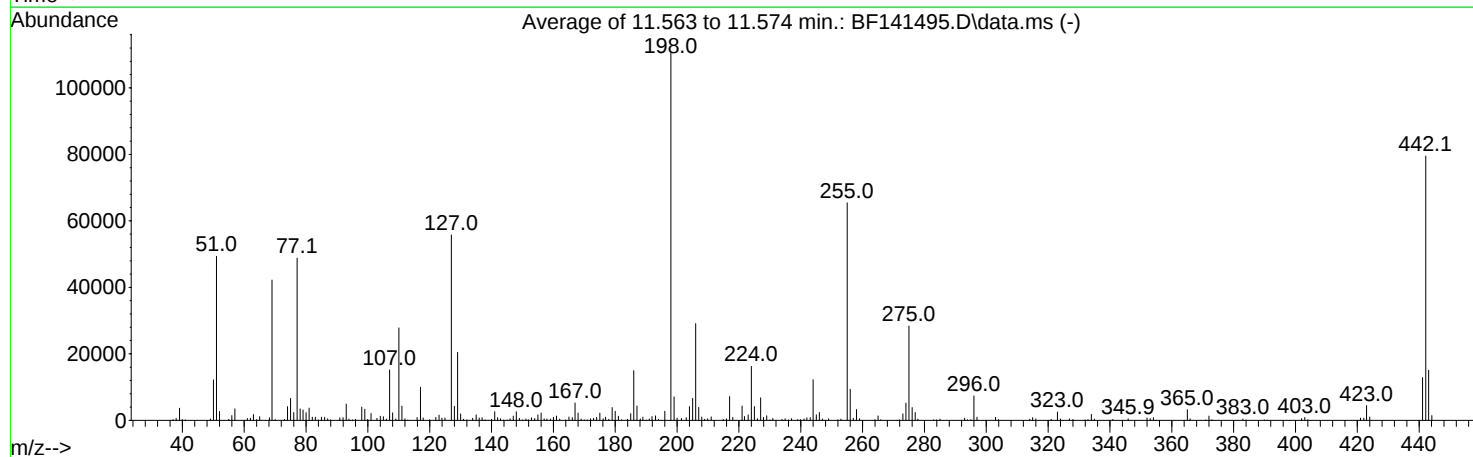


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141495.D
Acq On : 07 Feb 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

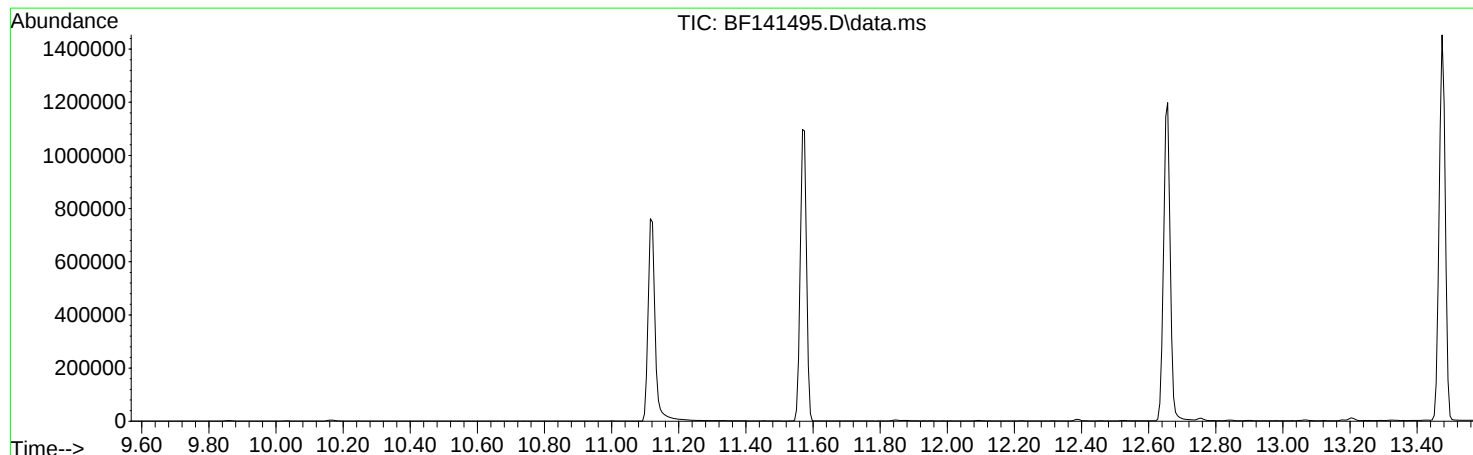

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	44.6	49336	PASS
68	69	0.00	2	1.9	790	PASS
69	198	0.00	100	38.1	42197	PASS
70	69	0.00	2	0.6	242	PASS
127	198	10	80	50.4	55765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	110645	PASS
199	198	5	9	6.4	7093	PASS
275	198	10	60	25.6	28376	PASS
365	198	1	100	2.9	3250	PASS
441	198	0.01	100	11.6	12847	PASS
442	442	50	100	100.0	79493	PASS
443	442	15	24	19.0	15087	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/7/2025	BNA_F	<u>BF141495.D</u>
Compound Name	Response	Retention Time
DDT	358775	13.474
DDD	5510	13.204
DDE	1622	12.657
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7132	365907	1.95

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141495.D
Acq On : 07 Feb 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 10:34:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

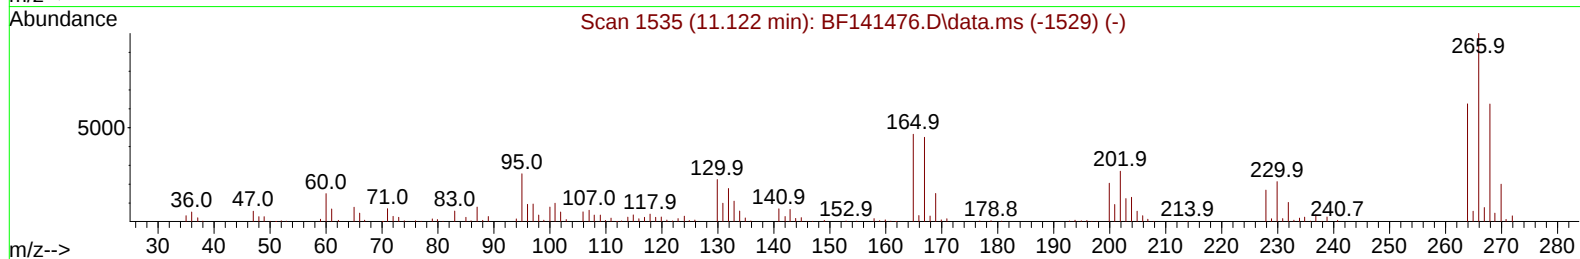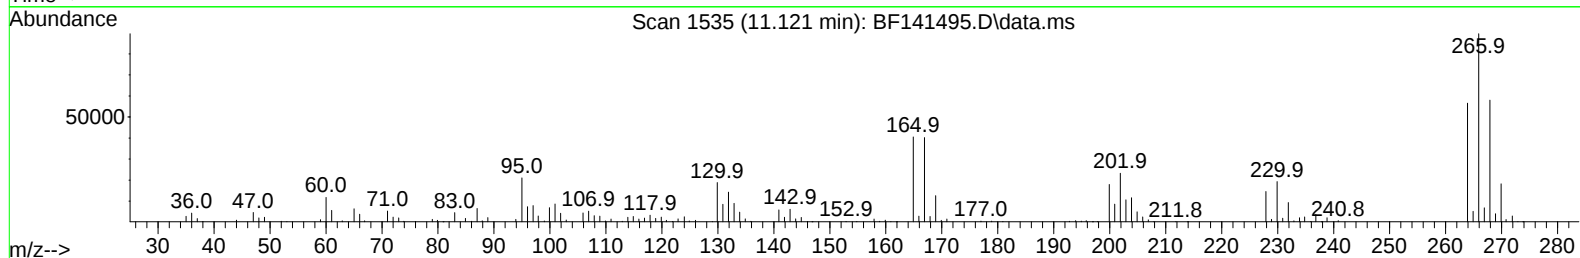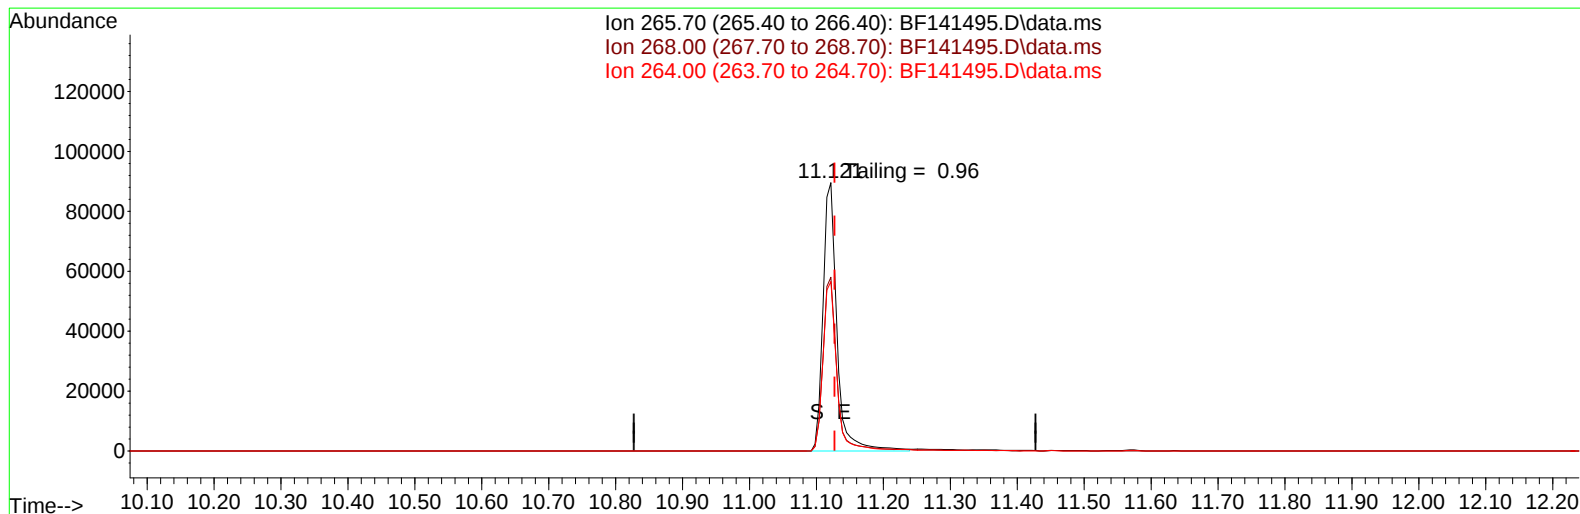

TIC: BF141495.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.006) 48103.02 ng




response 130265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.78
264.00	62.60	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141495.D
Acq On : 07 Feb 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 10:34:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

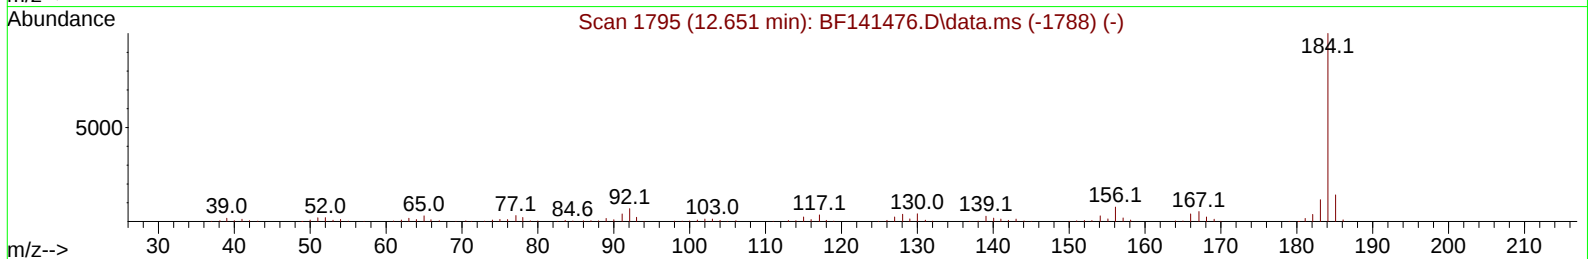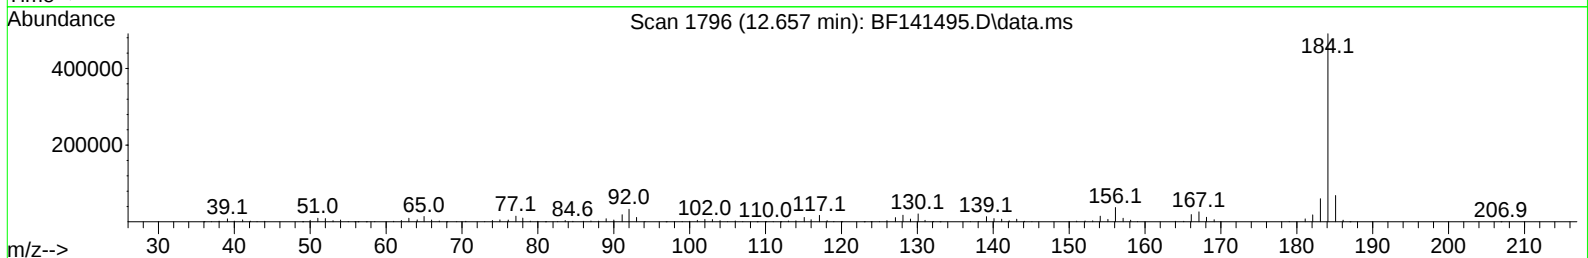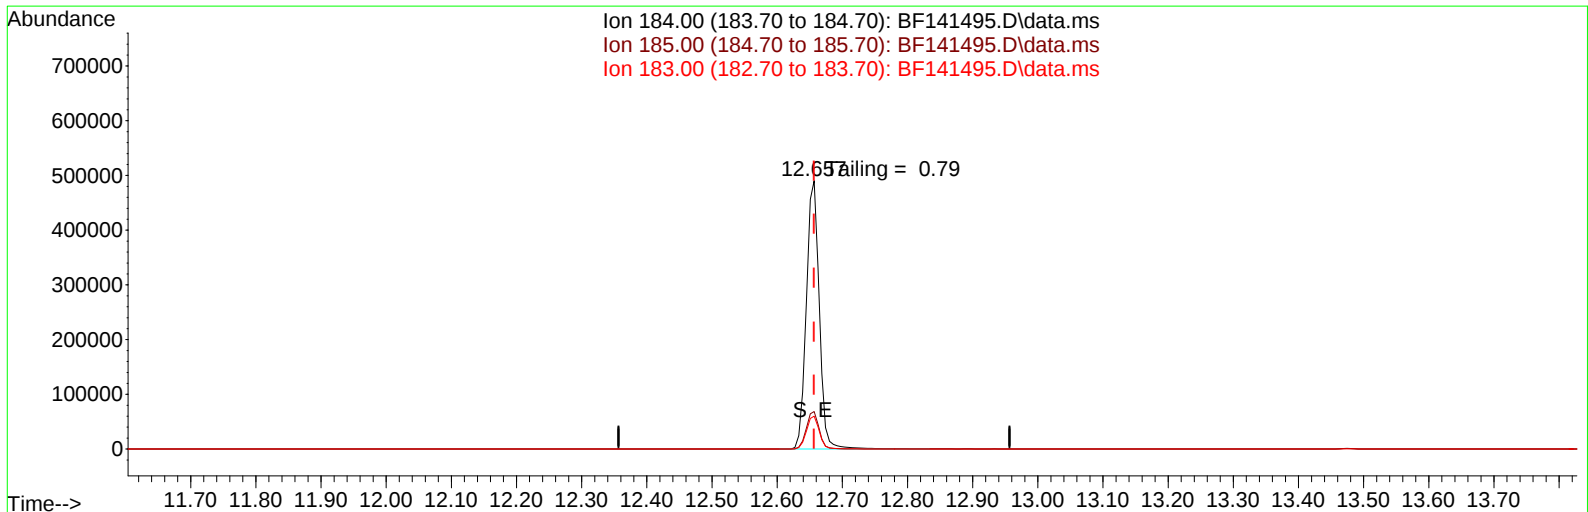

TIC: BF141495.D\data.ms

(77) Benzidine

12.657min (-0.000) 202039.83 ng

response 677290

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.96
183.00	11.60	12.26
0.00	0.00	0.00