
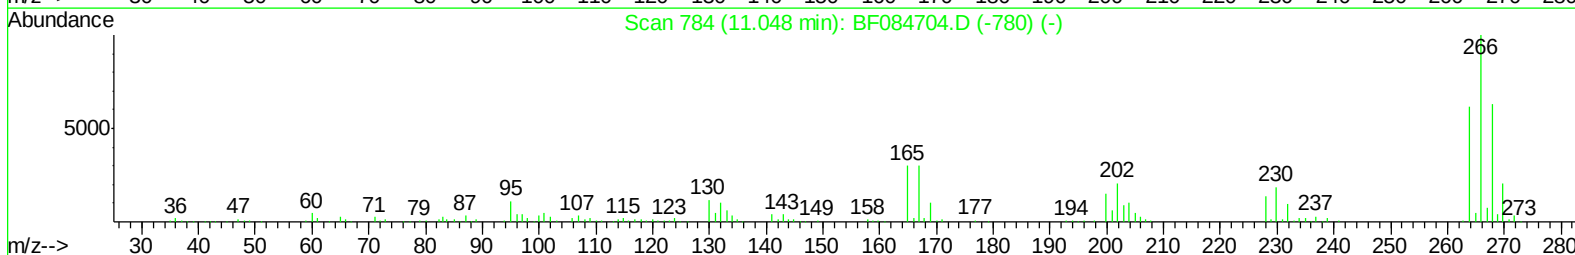
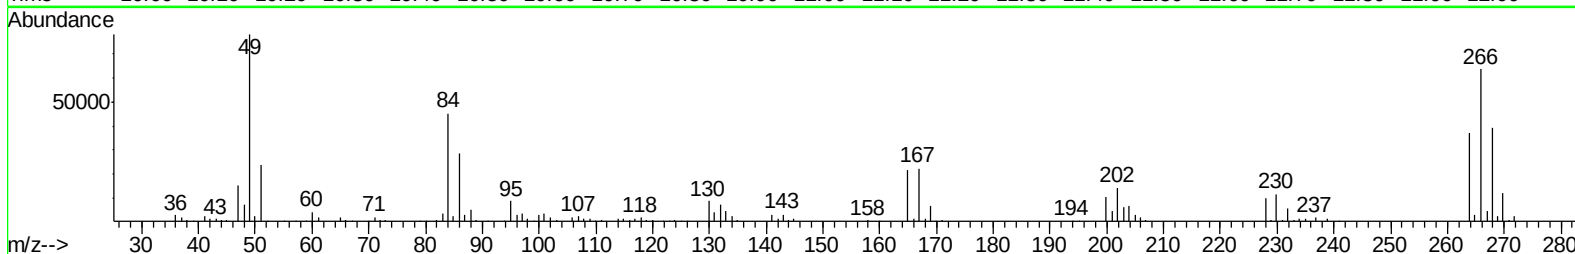


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
Data File : BF084926.D
Acq On : 8 Feb 2016 10:26
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 10:52:50 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

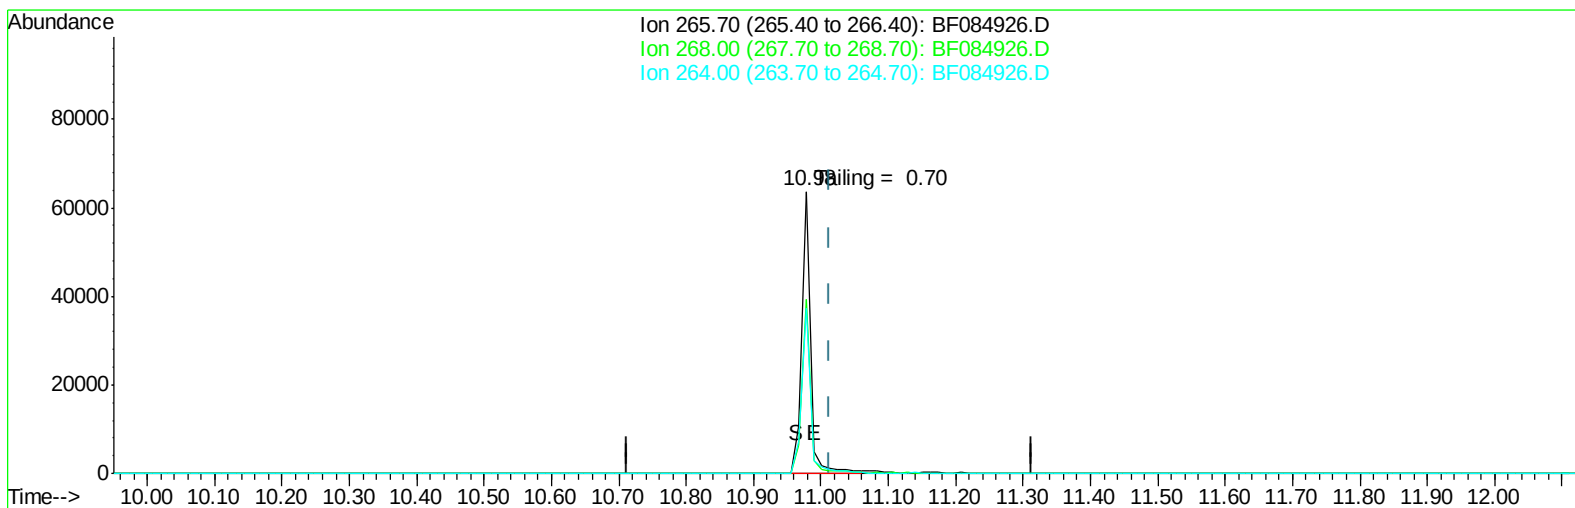

TIC: BF084926.D

(69) Pentachlorophenol (C)




10.979min (-0.034) 20550.26ng

response 59743

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.66
264.00	62.70	58.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
Data File : BF084926.D
Acq On : 8 Feb 2016 10:26
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 10:52:50 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

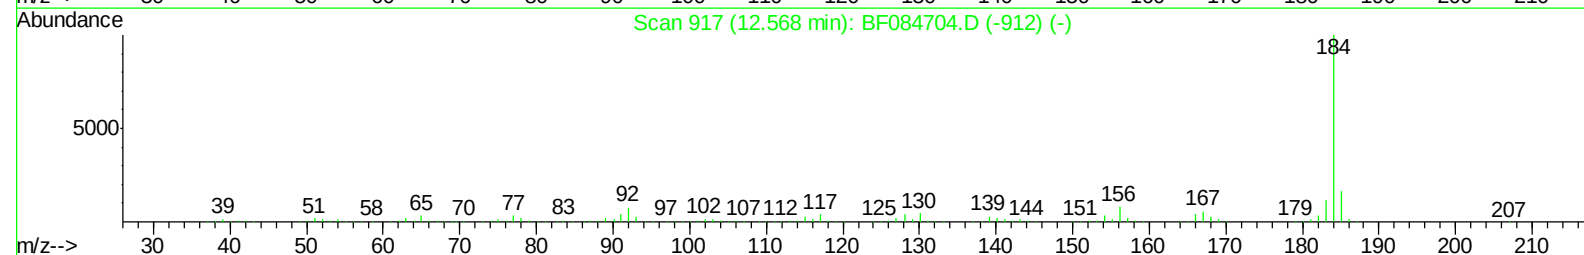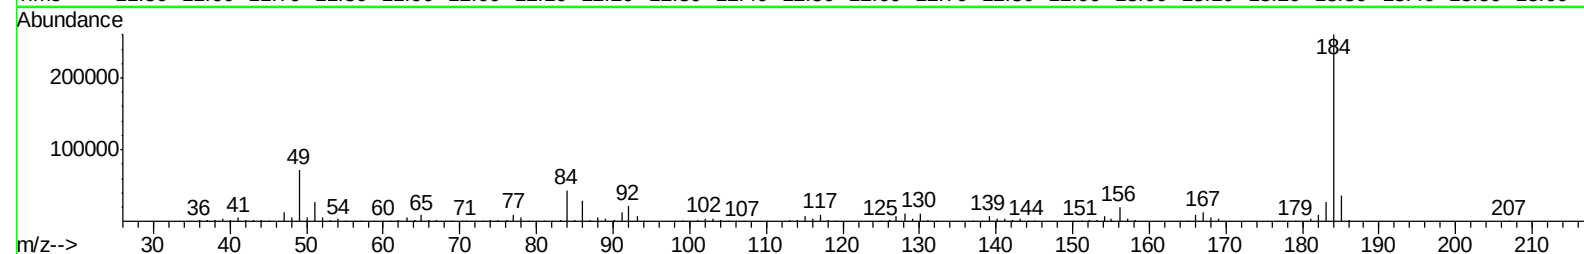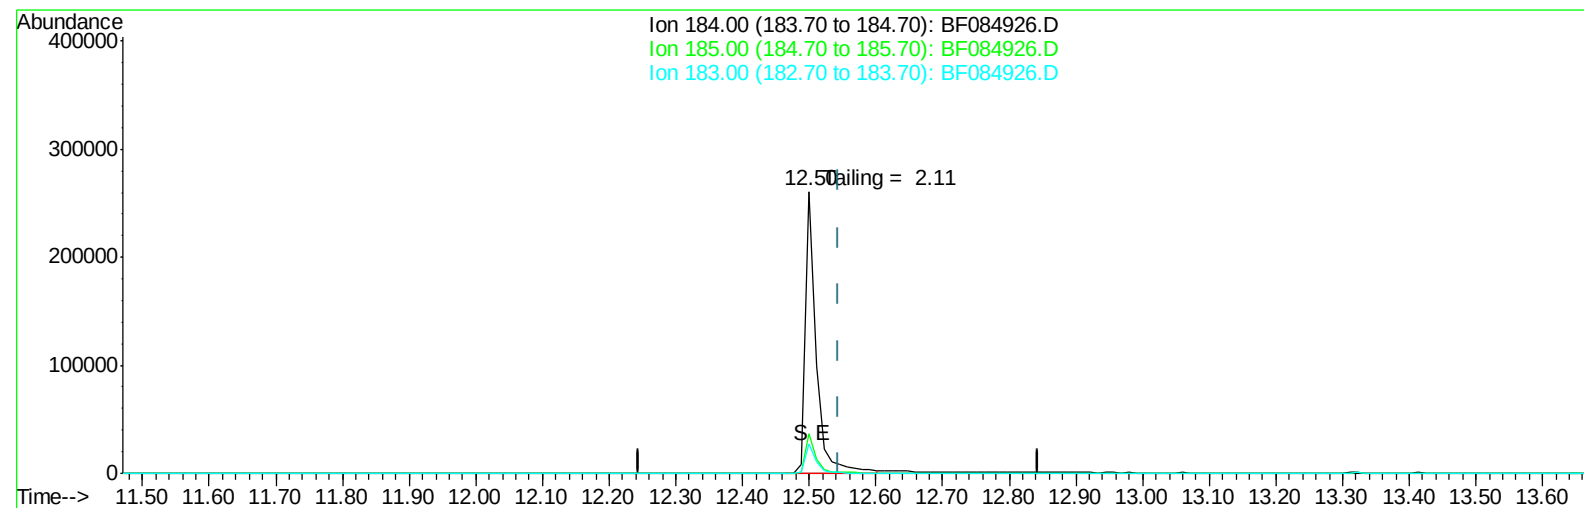

TIC: BF084926.D

(76) Benzidine

12.499min (-0.046) -20.00ng

response 303434

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.16
183.00	12.30	10.69
0.00	0.00	0.00