

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
 Data File : BF084941.D
 Acq On : 8 Feb 2016 21:06
 Operator : SJ/IZ
 Sample : H1329-01 25X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S4-B007(1-2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.773	234	235	241	rVB	58396	69131	2.04%	0.590%
2	5.230	273	275	282	rVB	277287	268900	7.93%	2.295%
3	6.304	366	369	376	rVB	206703	274922	8.11%	2.346%
4	6.419	376	379	381	rBV	300439	281135	8.29%	2.399%
5	6.647	397	399	401	rBV	1231059	1048720	30.93%	8.951%
6	6.807	410	413	415	rBV	158933	213209	6.29%	1.820%
7	7.219	446	449	451	rBV	149251	162348	4.79%	1.386%
8	7.939	509	512	514	rBV	1562318	1422762	41.96%	12.143%
9	9.013	604	606	608	rBV	403556	314705	9.28%	2.686%
10	9.688	662	665	667	rBV	1531991	1423552	41.98%	12.150%
11	10.465	731	733	736	rBV	147934	142300	4.20%	1.215%
12	11.162	791	794	796	rBV	1496500	1296502	38.23%	11.066%
13	12.362	898	899	901	rBV	50342	56581	1.67%	0.483%
14	12.591	916	919	921	rBV	69760	72070	2.13%	0.615%
15	12.739	931	932	935	rVB	178205	204995	6.05%	1.750%
16	13.654	1009	1012	1016	rVB3	31766	62805	1.85%	0.536%
17	13.791	1021	1024	1027	rBV	3455777	3391098	100.00%	28.943%
18	14.294	1065	1068	1074	rBV5	15507	40137	1.18%	0.343%
19	14.785	1109	1111	1114	rBV	32511	56197	1.66%	0.480%
20	15.048	1131	1134	1137	rBV	25165	41654	1.23%	0.356%
21	15.105	1137	1139	1141	rBV	26208	44388	1.31%	0.379%
22	15.162	1141	1144	1146	rBV	531777	789374	23.28%	6.737%
23	15.574	1178	1180	1183	rVB	28070	39104	1.15%	0.334%




Sum of corrected areas: 11716589

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
Data File : BF084941.D
Acq On : 8 Feb 2016 21:06
Operator : SJ/IZ
Sample : H1329-01 25X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4-B007(1-2)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

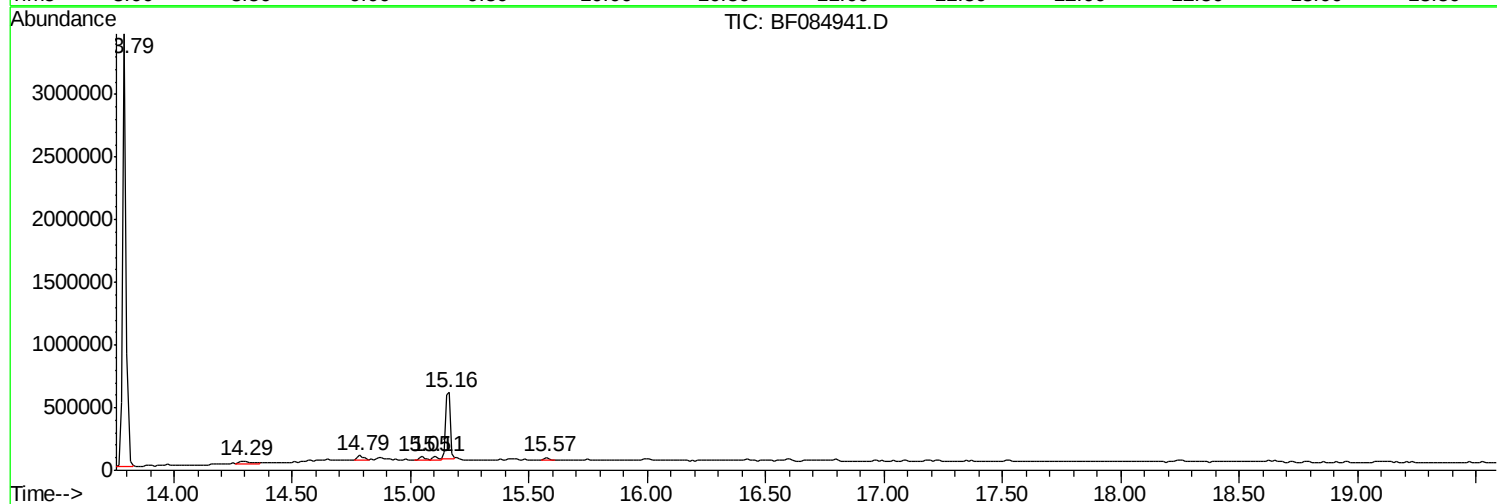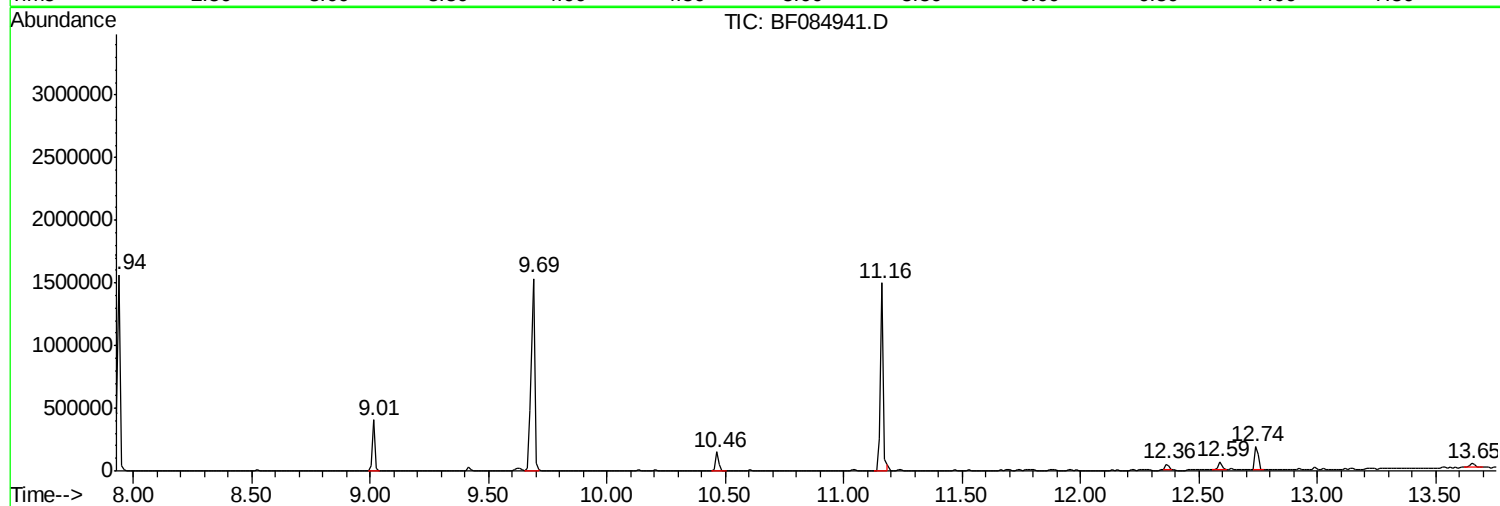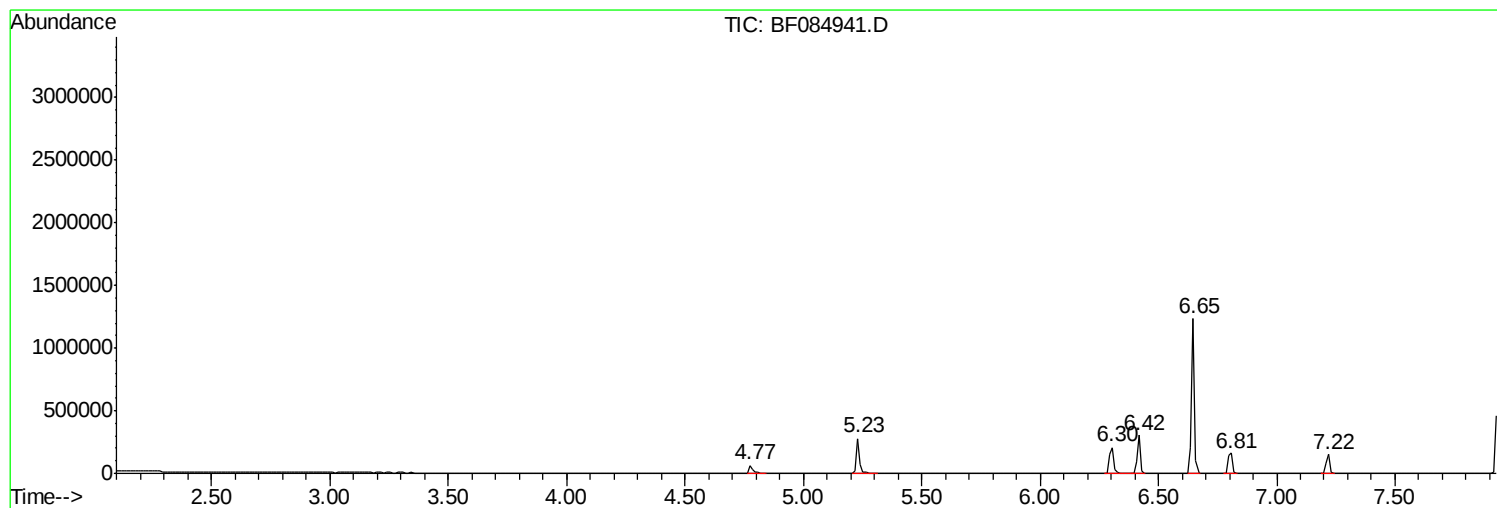

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
Data File : BF084941.D
Acq On : 8 Feb 2016 21:06
Operator : SJ/IZ
Sample : H1329-01 25X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4-B007(1-2)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	5.36 ng	281135	1,4-Dichlorobenzene-d4	6.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3			5-Aminoindole	132	C8H8N2	005192-03-0	12
4			(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	9
5			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

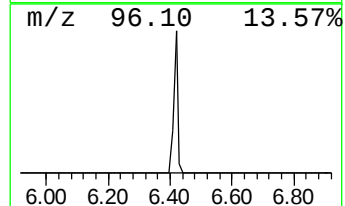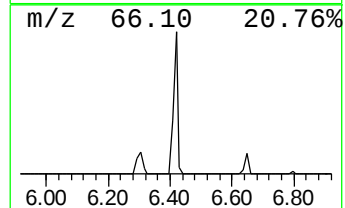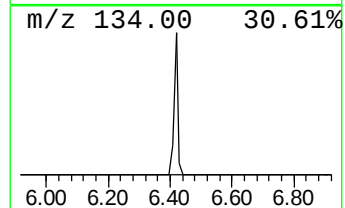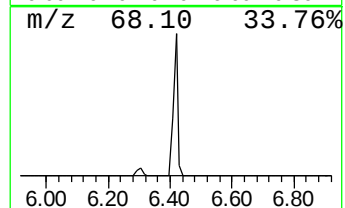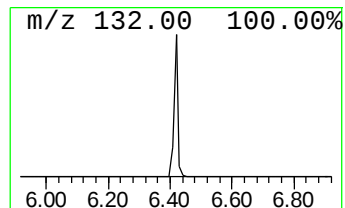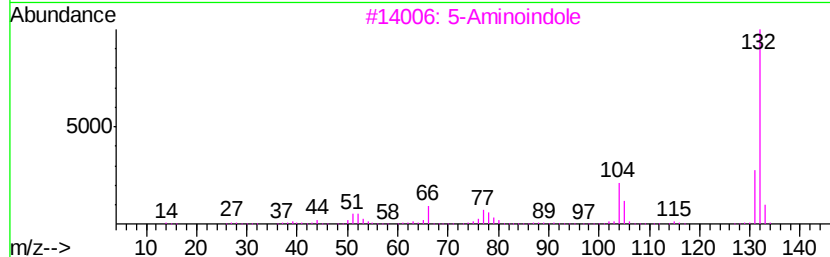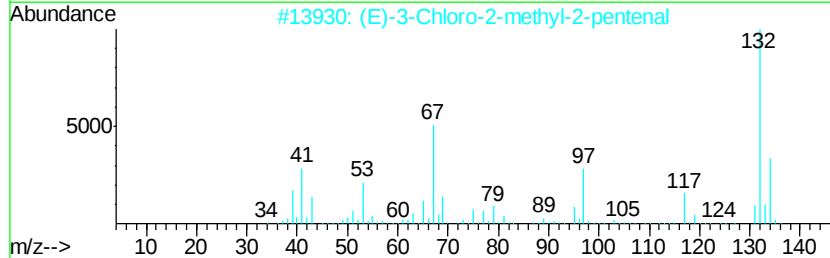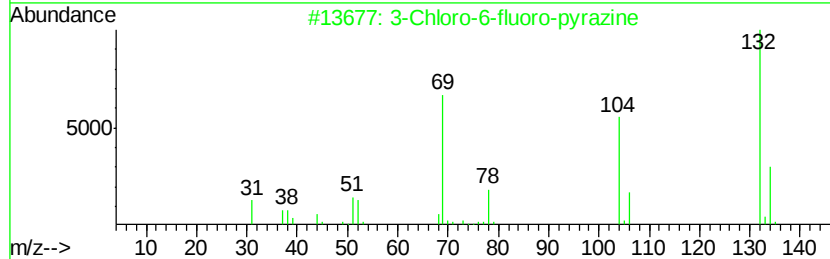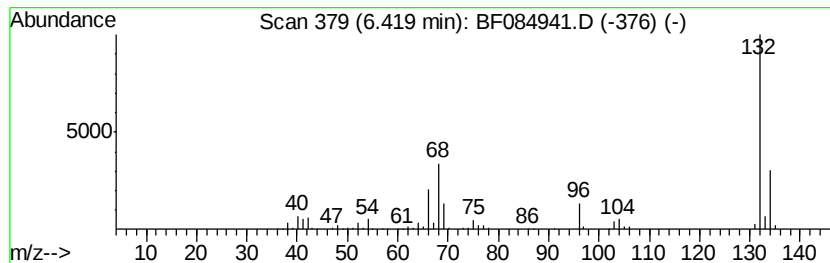

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
Data File : BF084941.D
Acq On : 8 Feb 2016 21:06
Operator : SJ/IZ
Sample : H1329-01 25X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4-B007(1-2)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	5.4	ng	281135	1	6.65	1048720	20.0