


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020816\
 Data File : BF084926.D
 Acq On : 8 Feb 2016 10:26
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 14:16:01 2016

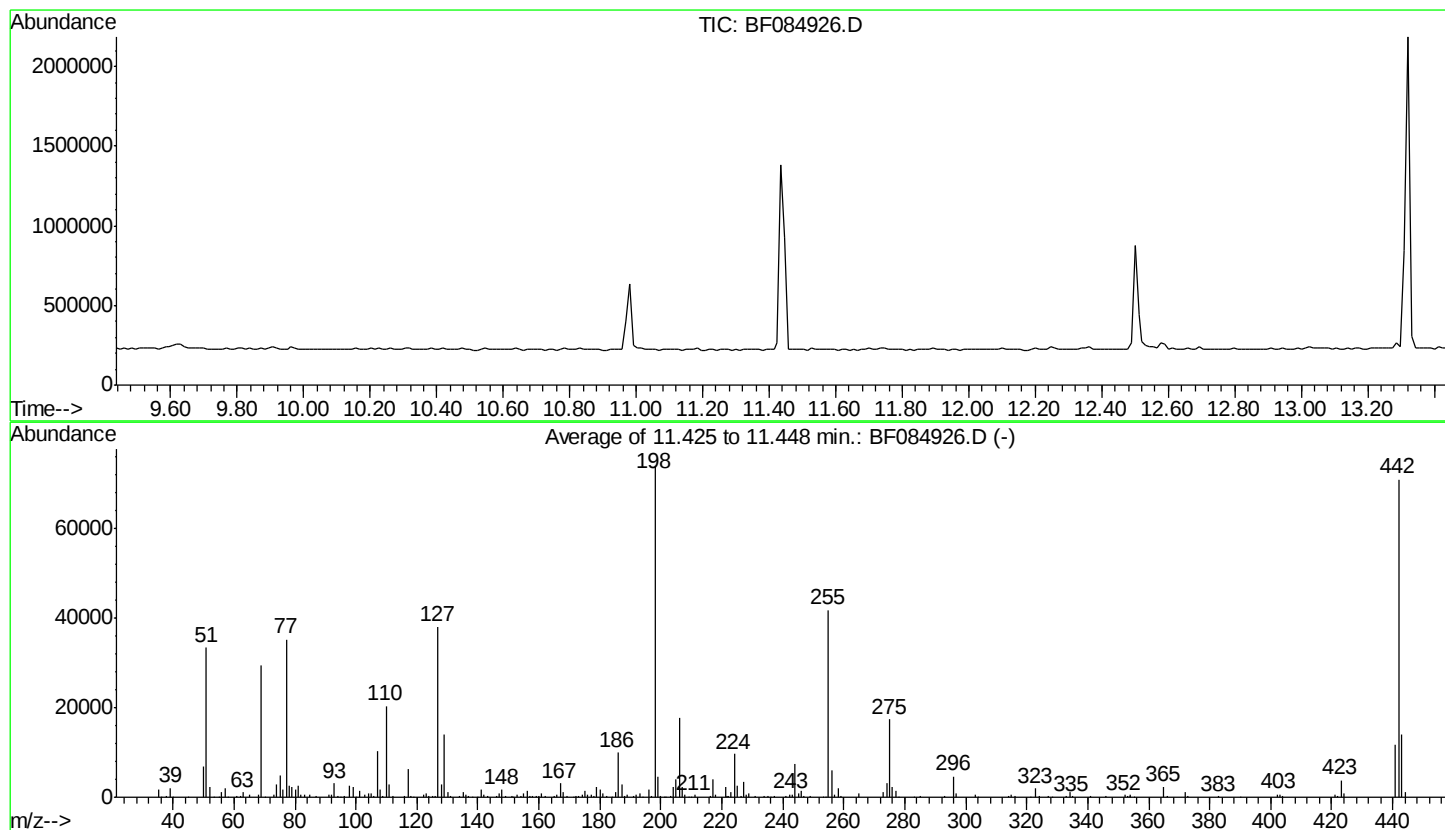

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	33418	PASS
68	69	0.00	2	1.5	447	PASS
69	198	0.00	100	39.8	29487	PASS
70	69	0.00	2	0.3	91	PASS
127	198	10	80	51.5	38142	PASS
197	198	0.00	2	0.4	272	PASS
198	198	100	100	100.0	74125	PASS
199	198	5	9	6.3	4704	PASS
275	198	10	60	23.5	17443	PASS
365	198	1	100	3.1	2303	PASS
441	442	0.01	24	16.5	11710	PASS
442	198	50	100	95.9	71073	PASS
443	442	15	24	19.5	13891	PASS