
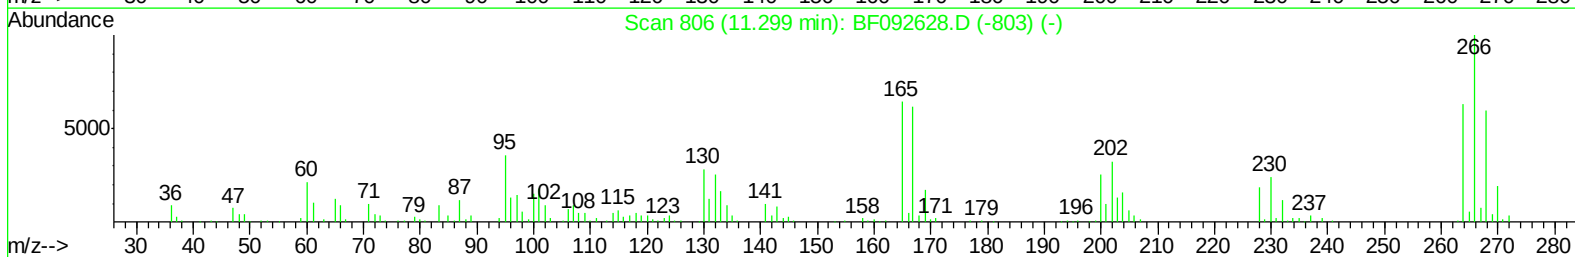
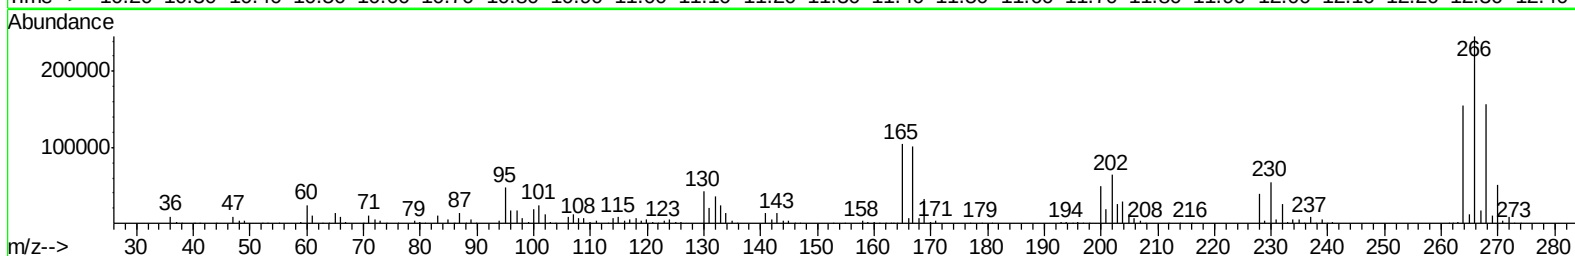


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020817\
Data File : BF092853.D
Acq On : 8 Feb 2017 14:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 03:40:53 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 23:48:40 2017
Response via : Initial Calibration

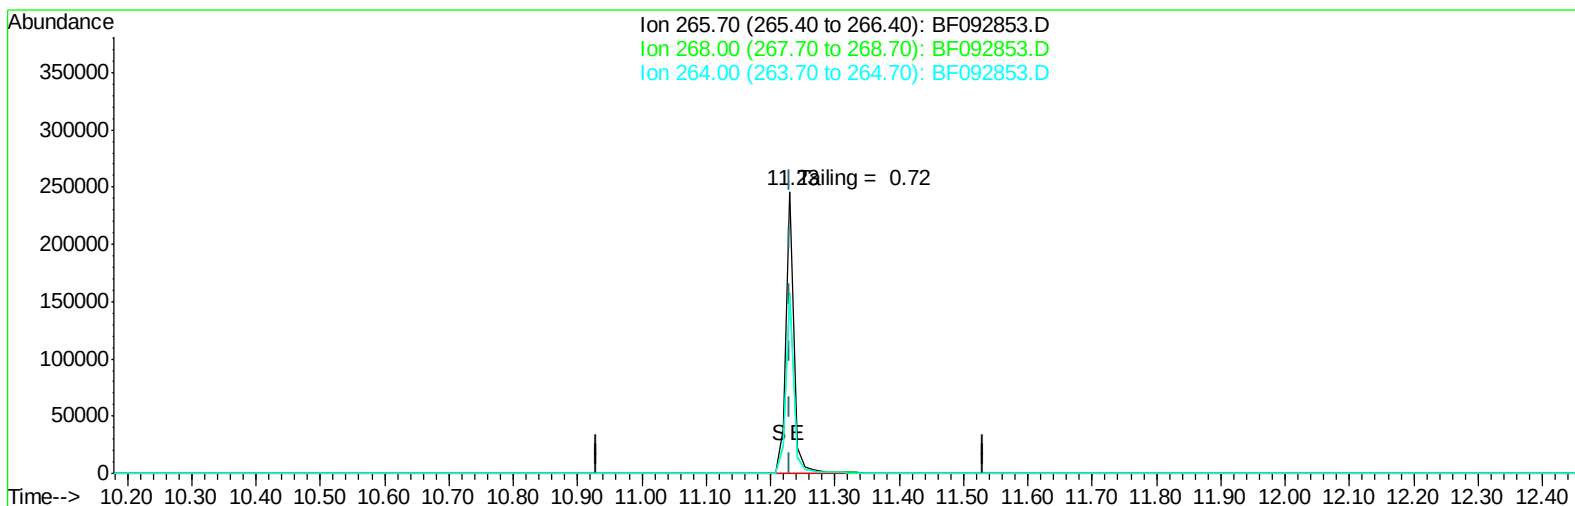

TIC: BF092853.D

(69) Pentachlorophenol (C)




11.231min (+0.000) 0.00ng

response 225580

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.06
264.00	62.90	62.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020817\
Data File : BF092853.D
Acq On : 8 Feb 2017 14:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 03:40:53 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 23:48:40 2017
Response via : Initial Calibration

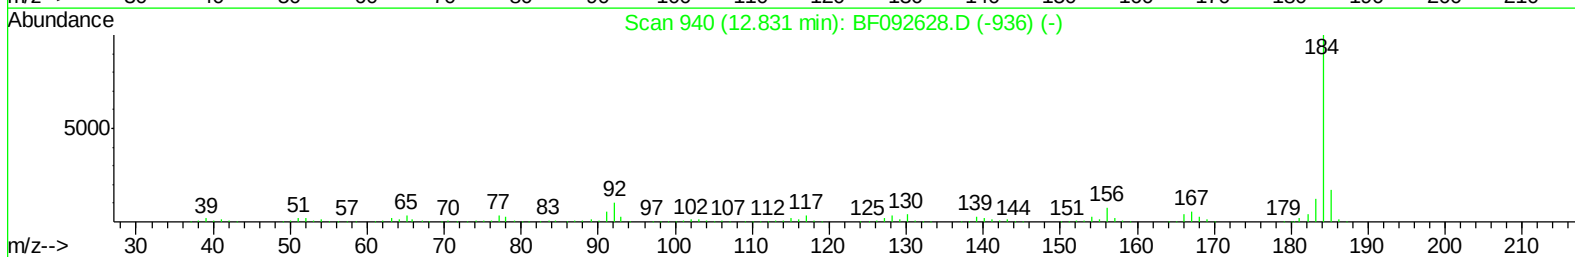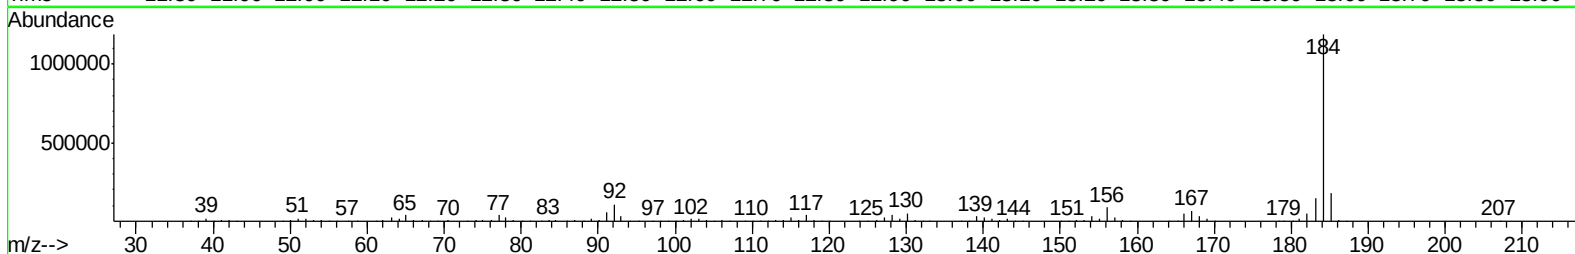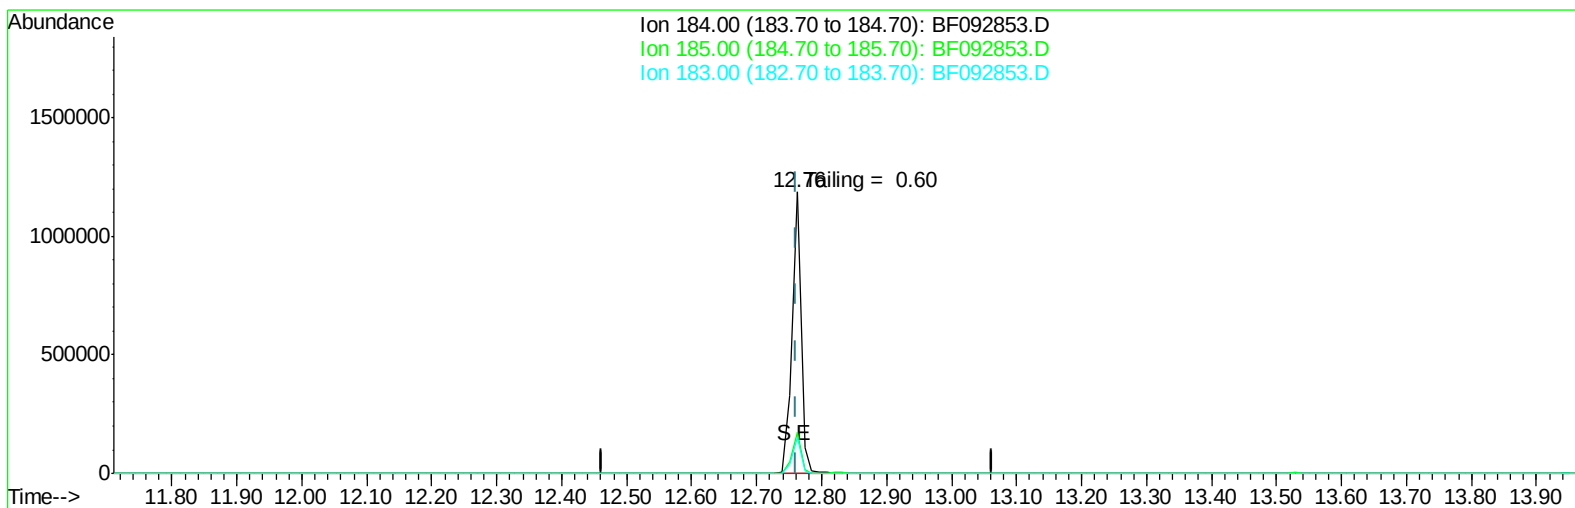

TIC: BF092853.D

(76) Benzidine

12.762min (+0.000) 59547.59ng

response 1141868

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.78
183.00	11.50	12.52
0.00	0.00	0.00