
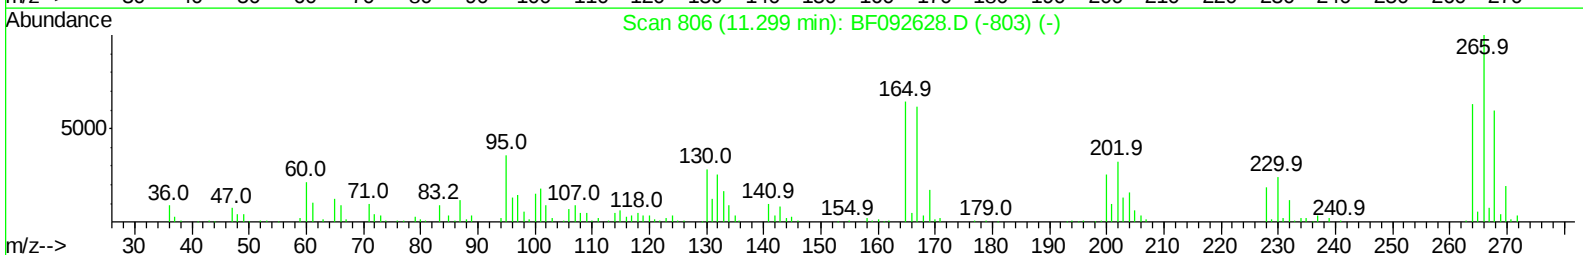
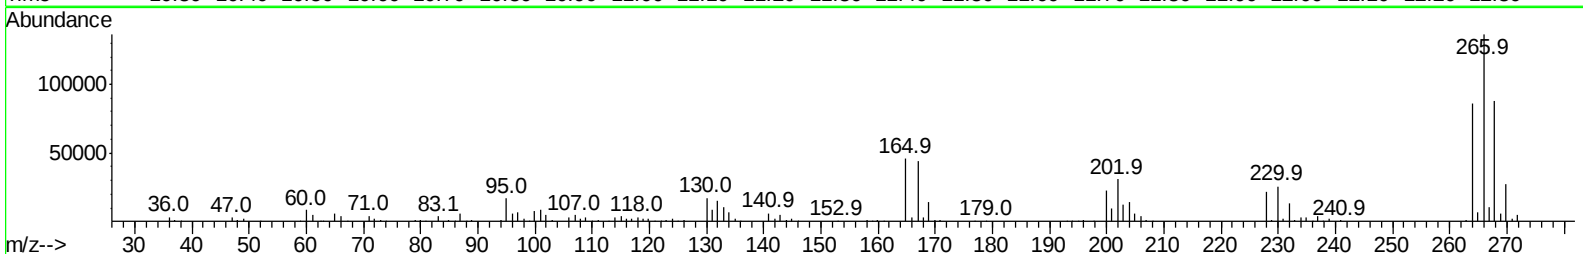


Data Path : Z:\HPCHEM1\BNA F\Data\BF020817\  
Data File : BF092878.D  
Acq On : 9 Feb 2017 10:21  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 17:53:44 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 30 14:50:05 2017  
Response via : Initial Calibration

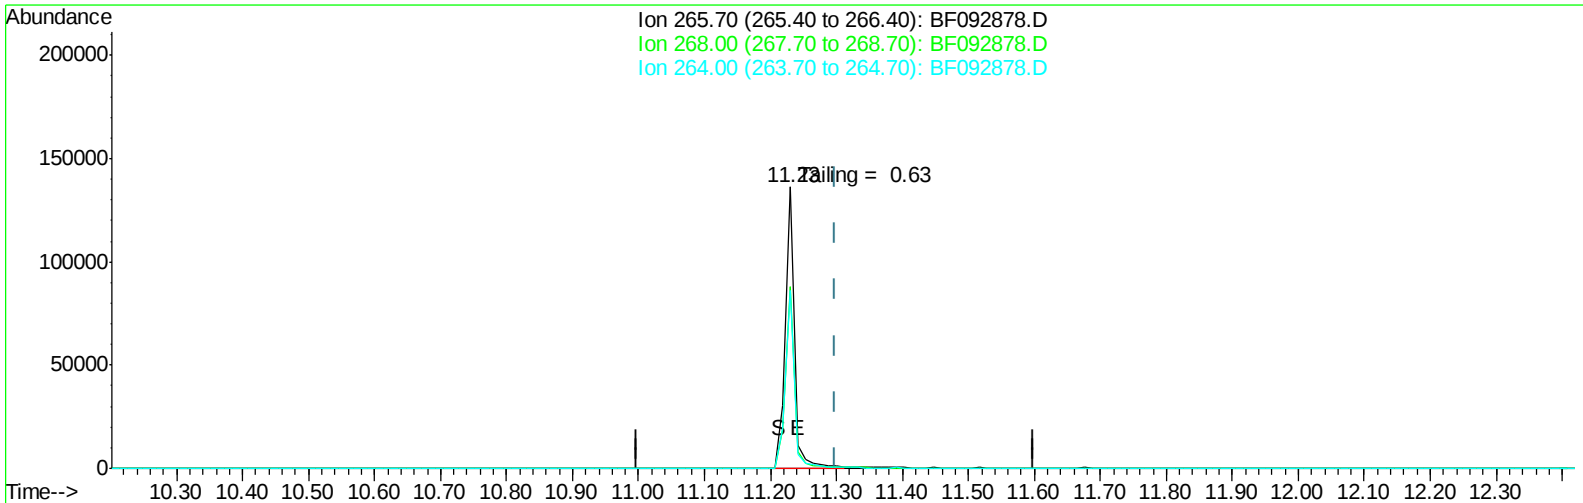

TIC: BF092878.D

(69) Pentachlorophenol (C)




11.230min (-0.069) 28235.63ng

response 133093

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.60 | 64.40 |
| 264.00 | 62.90 | 63.22 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\Data\BF020817\  
Data File : BF092878.D  
Acq On : 9 Feb 2017 10:21  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 17:53:44 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 30 14:50:05 2017  
Response via : Initial Calibration

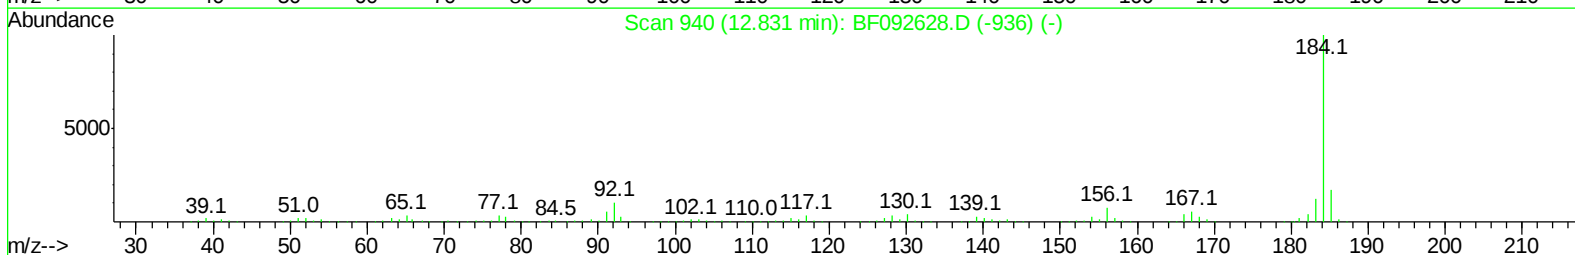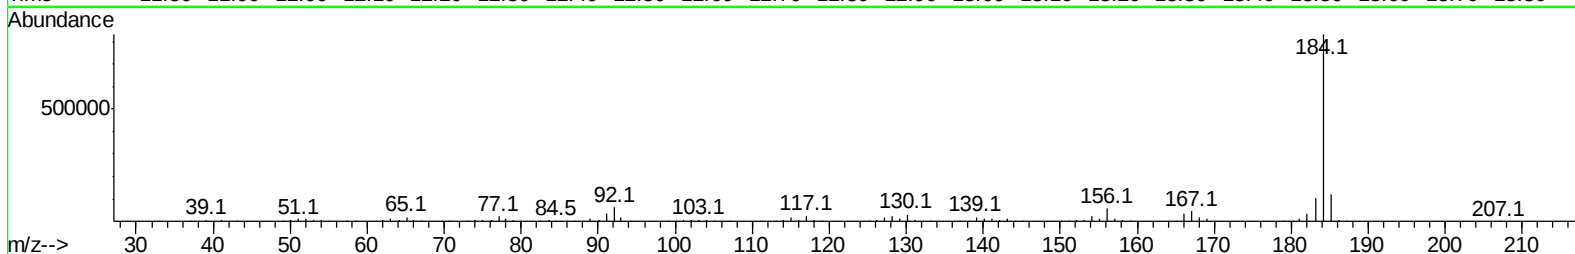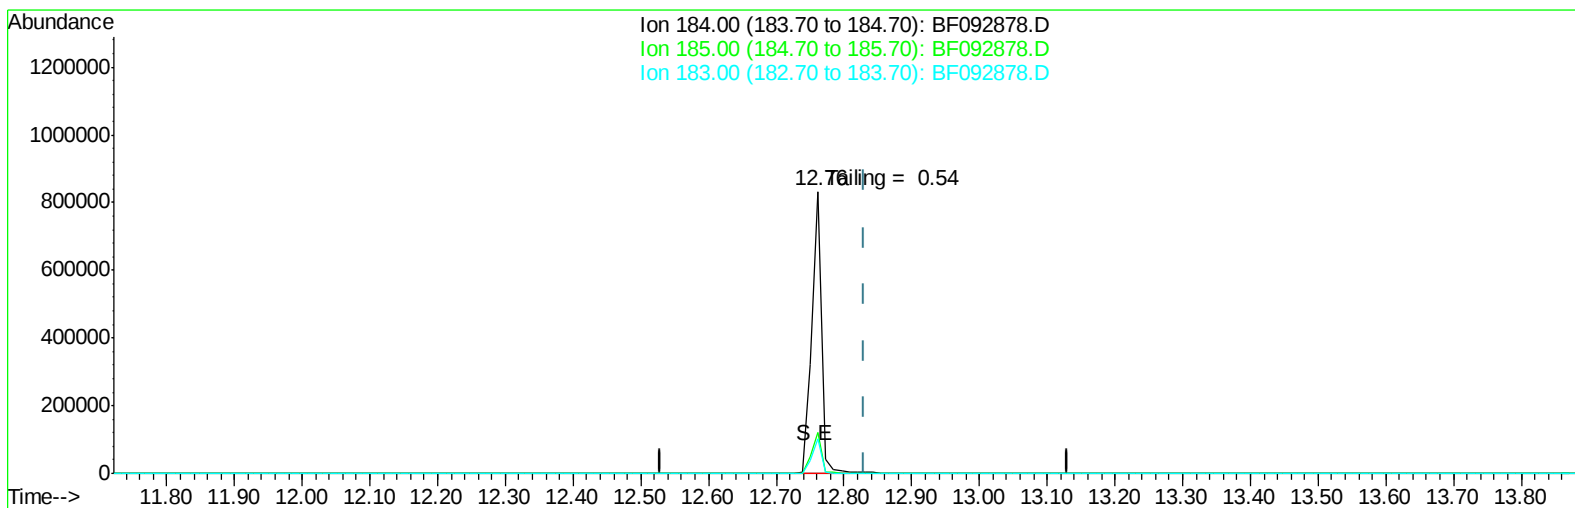

TIC: BF092878.D

(76) Benzidine

12.762min (-0.069) 14878.15ng

response 846388

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.70 | 14.54 |
| 183.00 | 11.50 | 12.49 |
| 0.00   | 0.00  | 0.00  |