
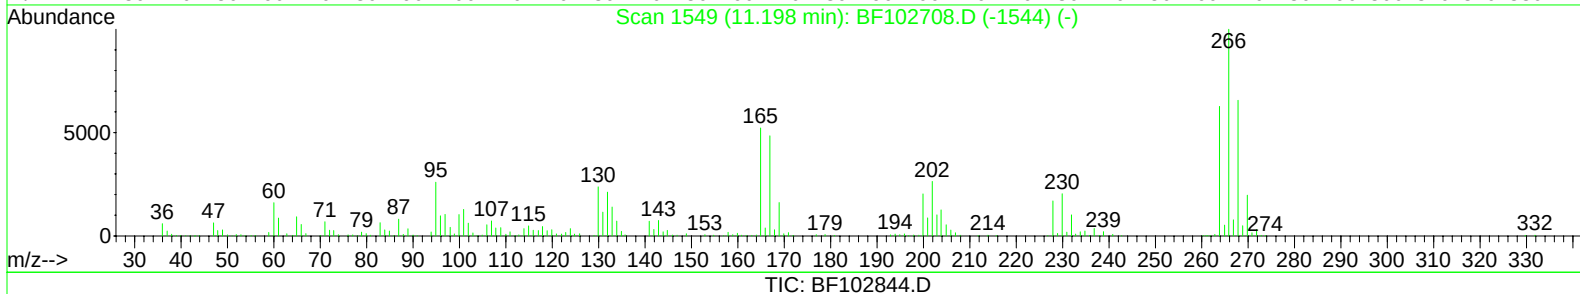
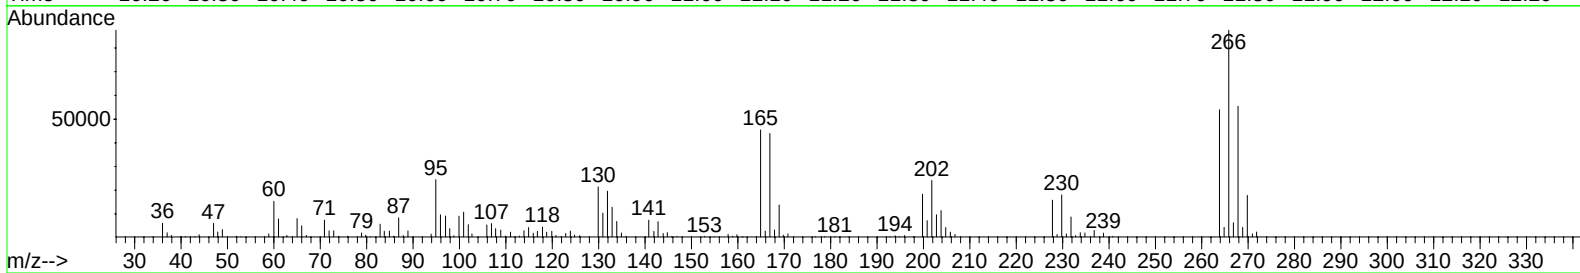


Data Path : Z:\HPCHEM1\BNA F\DATA\BF020818\  
Data File : BF102844.D  
Acq On : 8 Feb 2018 9:22  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 02:06:14 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 12:44:16 2018  
Response via : Initial Calibration

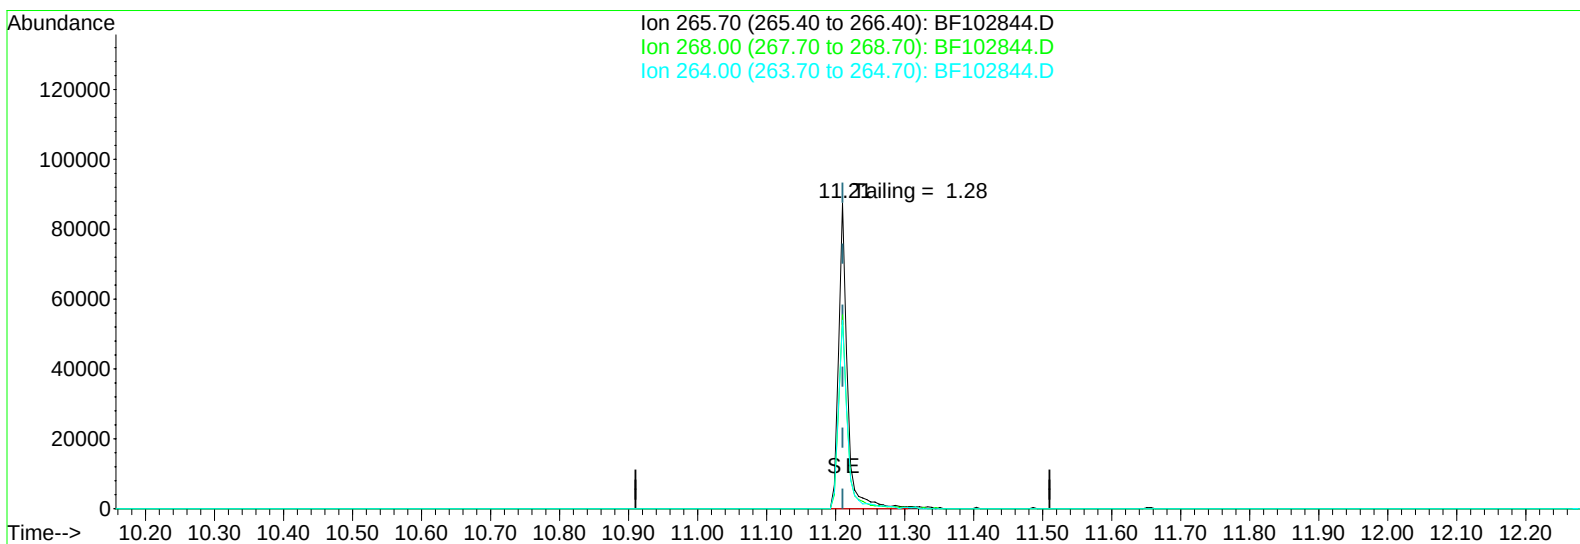

(69) Pentachlorophenol (C)




11.210min (+0.000) 24829.64ng

response 76711

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.36 |
| 264.00 | 61.90 | 61.61 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020818\  
Data File : BF102844.D  
Acq On : 8 Feb 2018 9:22  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 02:06:14 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 12:44:16 2018  
Response via : Initial Calibration

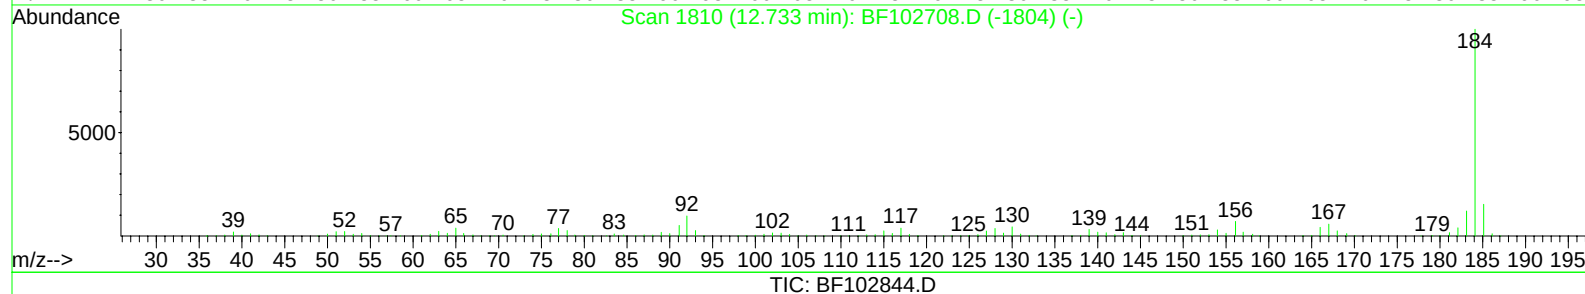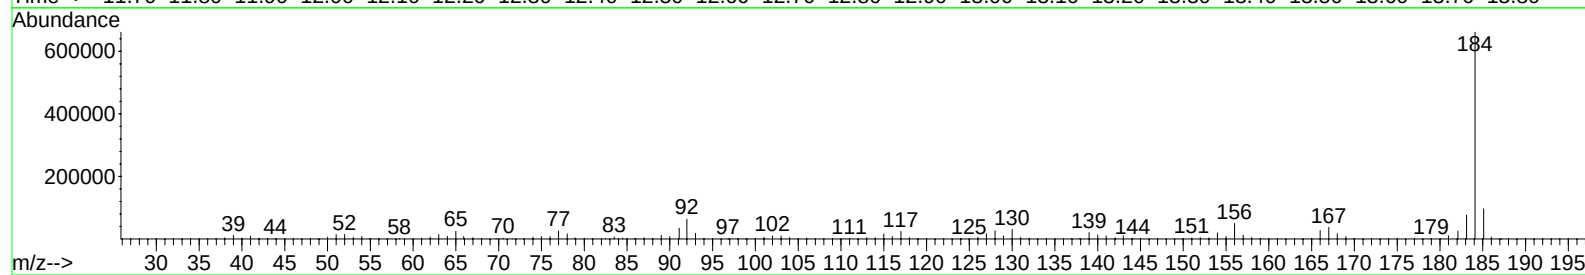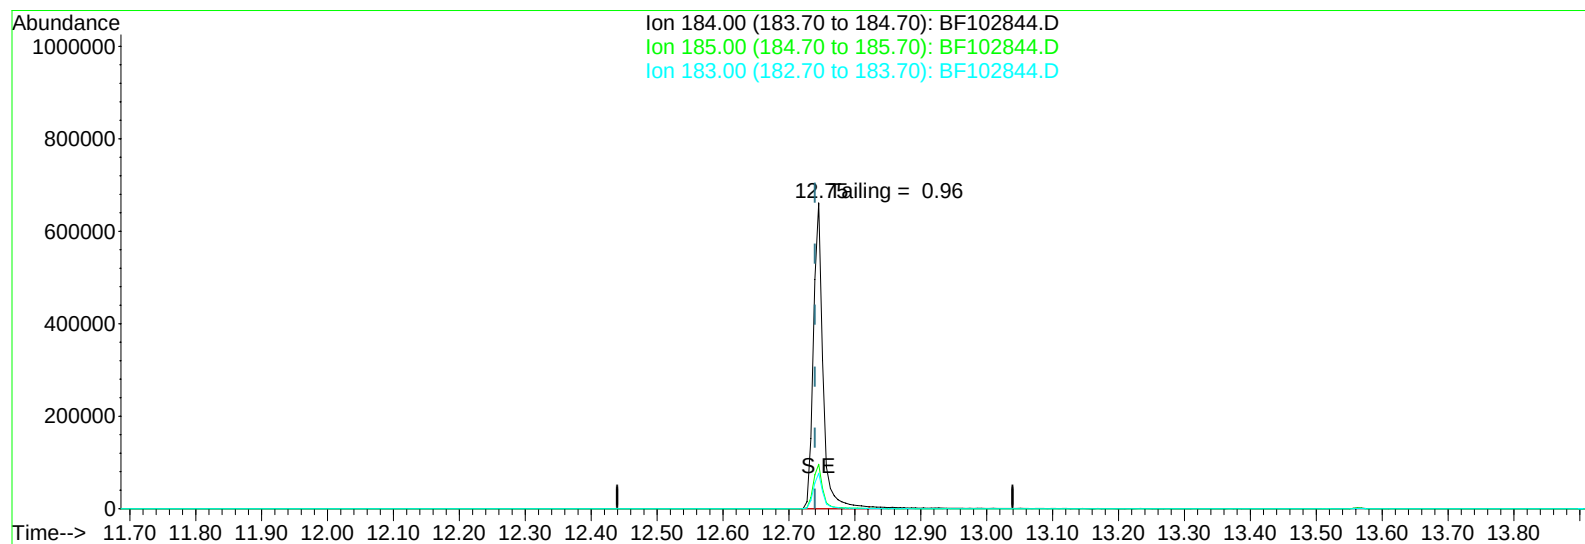

(76) Benzidine

12.745min (+0.006) 0.00ng

response 678923

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.54 |
| 183.00 | 11.60 | 11.58 |
| 0.00   | 0.00  | 0.00  |