
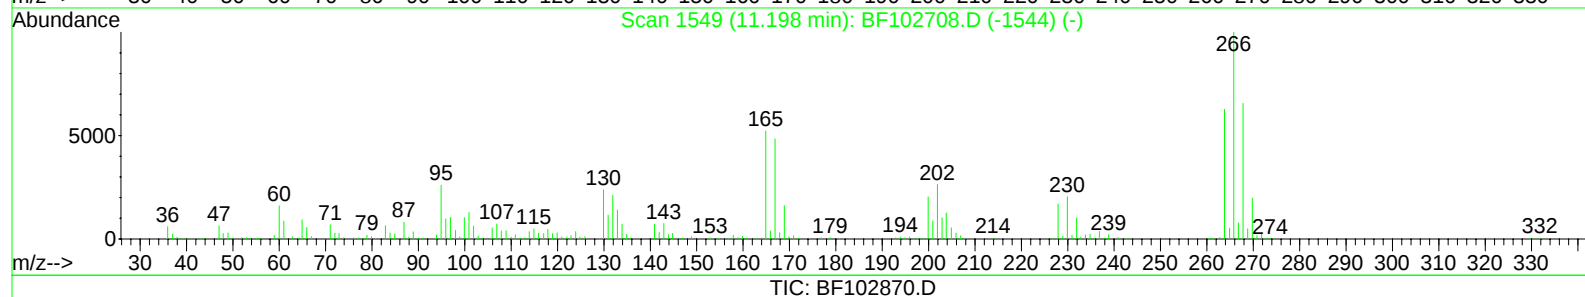
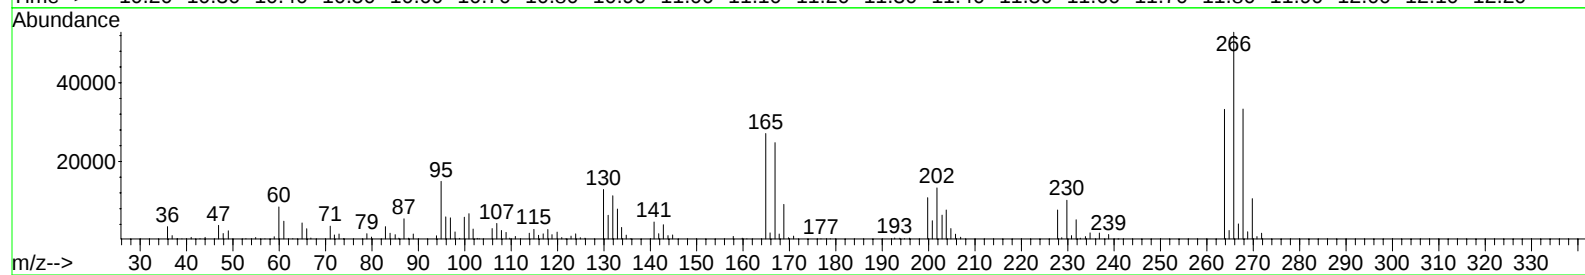


Data Path : Z:\HPCHEM1\BNA F\DATA\BF020818\
Data File : BF102870.D
Acq On : 8 Feb 2018 22:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 02:12:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

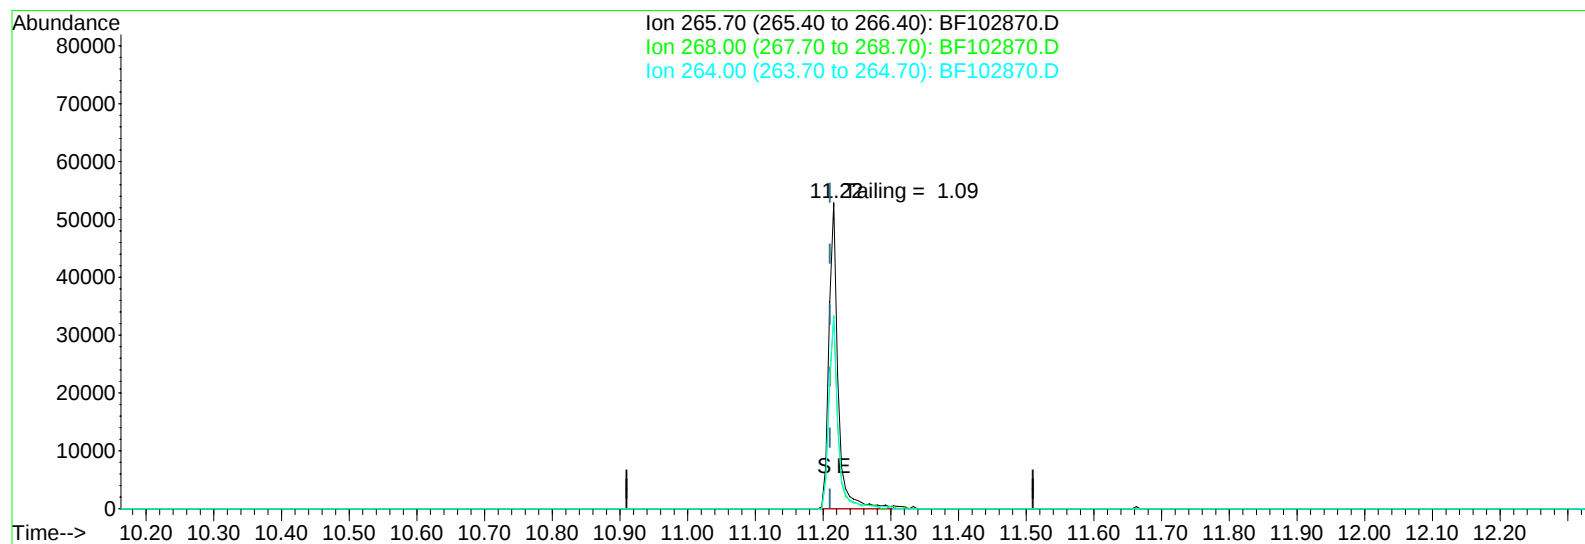

(69) Pentachlorophenol (C)




11.216min (+0.006) 49728.07ng

response 50076

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.04
264.00	61.90	62.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020818\
Data File : BF102870.D
Acq On : 8 Feb 2018 22:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 02:12:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

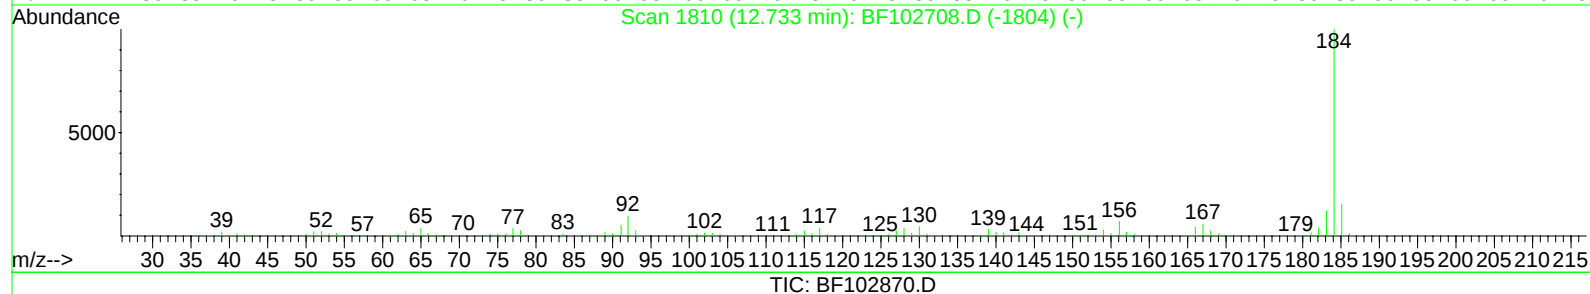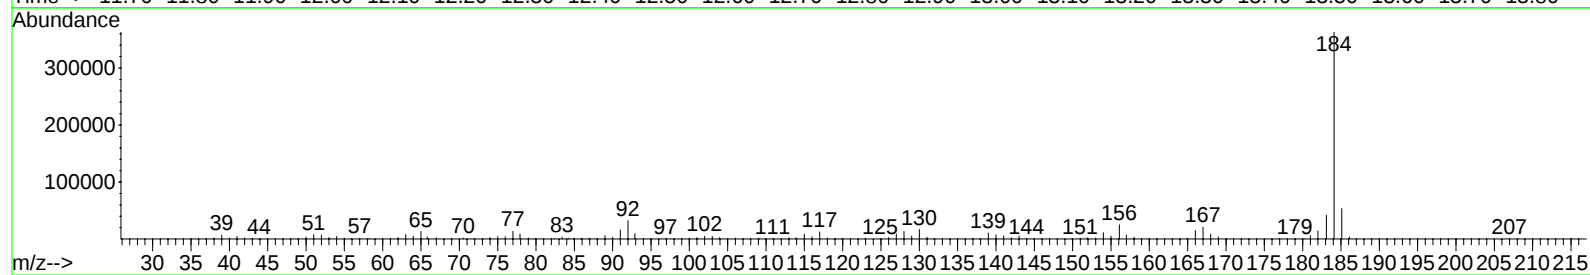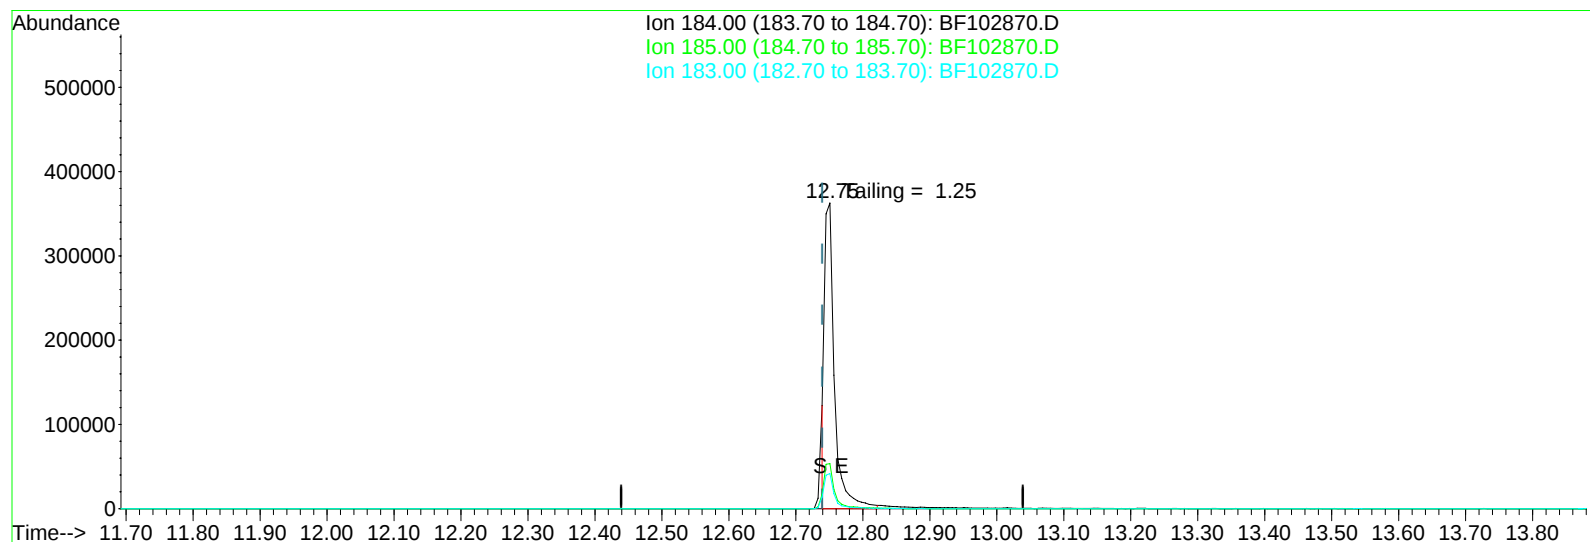

(76) Benzidine

12.751min (+0.012) 0.00ng

response 427617

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.72
183.00	11.60	11.49
0.00	0.00	0.00