


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020818\
 Data File : BF102844.D
 Acq On : 8 Feb 2018 9:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

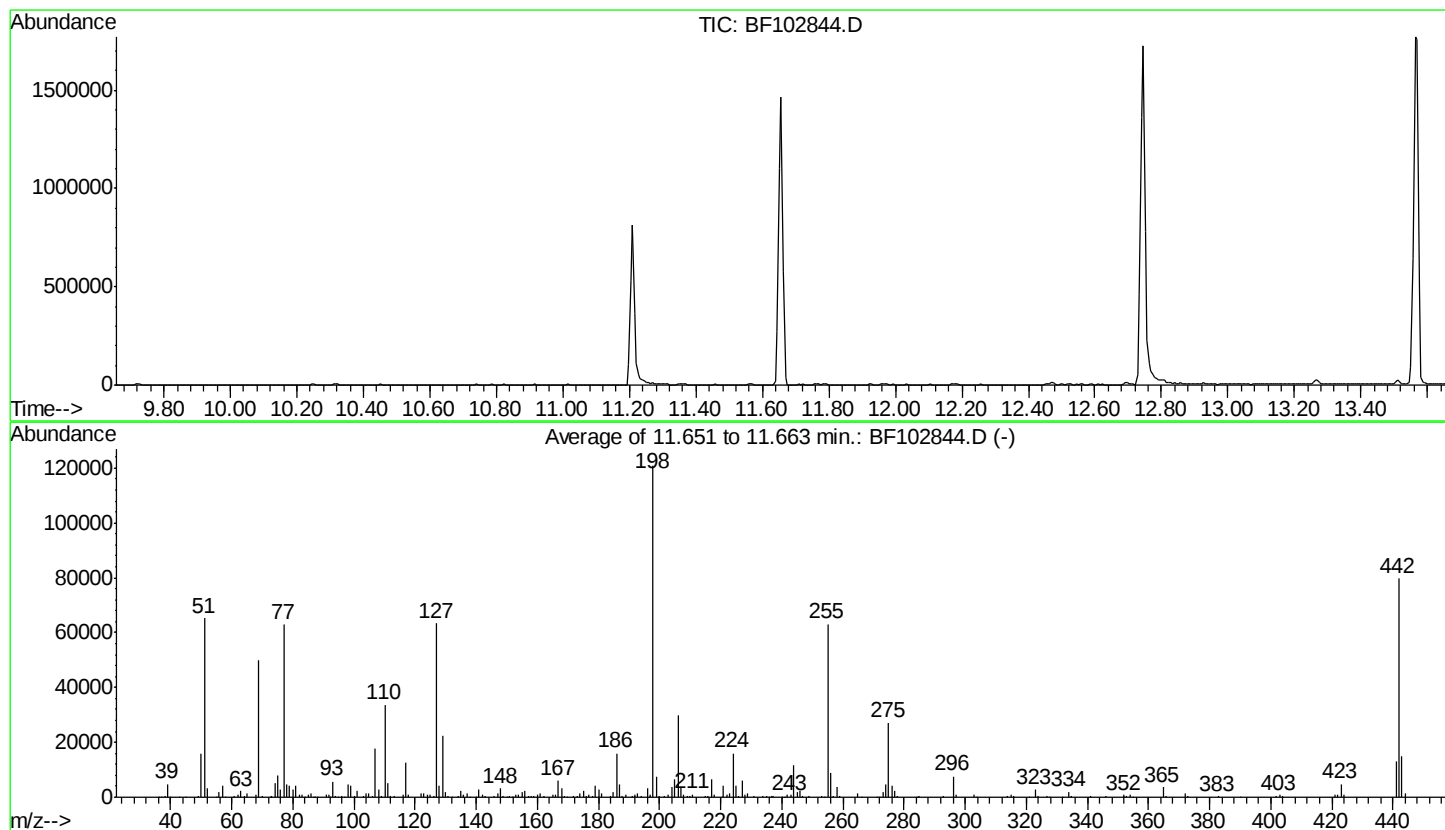

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.0	65250	PASS
68	69	0.00	2	1.9	941	PASS
69	198	0.00	100	41.2	49800	PASS
70	69	0.00	2	0.5	253	PASS
127	198	10	80	52.5	63434	PASS
197	198	0.00	2	0.9	1038	PASS
198	198	100	100	100.0	120890	PASS
199	198	5	9	6.1	7387	PASS
275	198	10	60	22.4	27082	PASS
365	198	1	100	3.0	3610	PASS
441	443	0.01	100	88.6	13315	PASS
442	198	50	100	66.0	79760	PASS
443	442	15	24	18.8	15026	PASS